

**EXHIBIT A  
FOLLOWS**



US008257305B2

(12) **United States Patent**  
**Speck et al.**

(10) **Patent No.:** **US 8,257,305 B2**  
(45) **Date of Patent:** **Sep. 4, 2012**

(54) **MEDICAL DEVICE FOR DISPENSING  
MEDICAMENTS**

(75) **Inventors:** **Ulrich Speck, Berlin (DE); Bruno  
Scheller, Saarbrücken (DE)**

(73) **Assignee:** **Bayer Pharma Aktiengesellschaft,  
Berlin (DE)**

(\*) **Notice:** Subject to any disclaimer, the term of this  
patent is extended or adjusted under 35  
U.S.C. 154(b) by 577 days.

4,247,352 A 1/1981 Stupp et al.  
4,305,926 A 12/1981 Everse et al.  
4,343,788 A 8/1982 Mustacich et al.  
4,364,921 A 12/1982 Speck et al.  
4,476,590 A 10/1984 Scales et al.  
4,479,795 A 10/1984 Mustacich et al.  
4,502,158 A 3/1985 Mouri et al.  
4,502,159 A 3/1985 Woodroof et al.  
4,532,315 A 7/1985 Letoffe et al.  
4,573,476 A 3/1986 Ruiz et al.  
4,677,143 A 6/1987 Laurin et al.  
4,769,013 A 9/1988 Lorenz et al.

(Continued)

#### FOREIGN PATENT DOCUMENTS

(21) **Appl. No.:** **10/528,577**

CA 2 132 936 AA 3/1995

(22) **PCT Filed:** **Aug. 26, 2003**

(Continued)

(86) **PCT No.:** **PCT/DE03/02871**

§ 371 (c)(1),  
(2), (4) **Date:** **Mar. 21, 2005**

#### OTHER PUBLICATIONS

(87) **PCT Pub. No.:** **WO2004/028582**

**PCT Pub. Date:** **Apr. 8, 2004**

Pierre Signore et al., "Complete Inhibition of Intimal Hyperplasia by  
Perivascular Delivery of Paclitaxel in Balloon-injured Rat Carotid  
Arteries," *Laboratory Investigations*, vol. 12, No. 1, Jan. 2001, pp.  
79-88.

(Continued)

(65) **Prior Publication Data**

US 2006/0020243 A1 Jan. 26, 2006

*Primary Examiner* — Laura Bouchelle

(30) **Foreign Application Priority Data**

Sep. 20, 2002 (DE) ..... 102 44 847

(74) *Attorney, Agent, or Firm* — Millen, White, Zelano &  
Branigan, P.C.

(51) **Int. Cl.**

**A61M 29/00** (2006.01)

(57) **ABSTRACT**

(52) **U.S. Cl.** ..... 604/103.02; 623/1.11

(58) **Field of Classification Search** ..... 623/1.11;  
604/103.02

See application file for complete search history.


For selective treatment of diseased tissue sections or organ  
parts, the surface of medical devices entering into contact  
with areas thereof under pressure is coated with lipophilic  
substantially water-insoluble medicaments binding to vari-  
ous tissue components with good adherence thereto, said  
medicaments having an effect thereupon a short time after  
entering into contact therewith without exerting a harmful  
influence upon adjacent healthy tissue.

(56) **References Cited**

#### U.S. PATENT DOCUMENTS

4,101,984 A 7/1978 MacGregor  
4,217,894 A 8/1980 Franetzki et al.

60 Claims, 1 Drawing Sheet

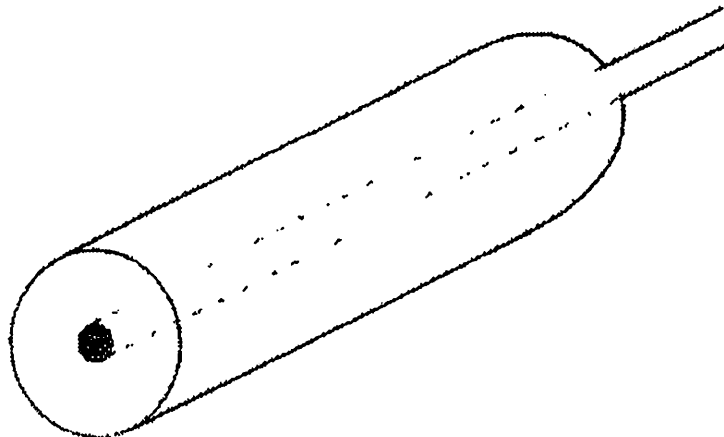

## US 8,257,305 B2

Page 2

## U.S. PATENT DOCUMENTS

4,776,337 A	10/1988	Palmaz et al.	5,607,475 A	3/1997	Cahalan et al.
4,793,825 A	12/1988	Benjamin et al.	5,609,629 A	3/1997	Fearnot et al.
4,872,867 A	10/1989	Joh	5,624,411 A	4/1997	Tuch
4,879,135 A	11/1989	Greco et al.	5,626,562 A	5/1997	Castro
4,886,062 A	12/1989	Wiktor	5,629,008 A	5/1997	Lee
4,909,799 A	3/1990	Thulesius et al.	5,629,881 A	5/1997	Leeb et al.
4,917,686 A	4/1990	Bayston et al.	5,643,580 A	7/1997	Subramaniam et al.
4,925,668 A	5/1990	Khan et al.	5,649,977 A	7/1997	Campbell et al.
4,950,256 A	8/1990	Luther et al.	5,674,192 A	10/1997	Sahatjian
4,994,047 A	2/1991	Walker et al.	5,679,400 A	10/1997	Tuch
4,997,643 A	3/1991	Partain et al.	5,681,846 A	10/1997	Trissel
5,004,461 A	4/1991	Wilson et al.	5,693,014 A	12/1997	Abele et al.
5,019,096 A	5/1991	Fox, Jr. et al.	5,697,967 A	12/1997	Dinh et al.
5,019,393 A	5/1991	Ito et al.	5,716,981 A	2/1998	Hunter et al.
5,019,601 A	5/1991	Allen	5,733,327 A	3/1998	Igaki et al.
5,051,257 A	9/1991	Pietronigro	5,762,638 A	6/1998	Shikani et al.
5,053,048 A	10/1991	Pinchuk	5,766,158 A	6/1998	Opolski
5,059,166 A	10/1991	Fischell et al.	5,770,198 A	6/1998	Coller et al.
5,067,491 A	11/1991	Taylor et al.	5,772,640 A	6/1998	Modak et al.
5,098,977 A	3/1992	Frautschi et al.	5,789,018 A	8/1998	Engelson et al.
5,102,402 A	4/1992	Dror et al. .... 604/265	5,792,158 A	8/1998	Lary
5,108,424 A	4/1992	Hoffman et al.	5,814,301 A	9/1998	Klopp et al.
5,112,457 A	5/1992	Marchant	5,820,607 A	10/1998	Tcholakian et al.
5,135,516 A	8/1992	Sahatjian et al.	5,824,049 A	10/1998	Ragheb et al.
5,157,049 A	10/1992	Haugwitz et al.	5,827,289 A	10/1998	Reiley
5,163,952 A	11/1992	Froix	5,837,008 A	11/1998	Berg et al.
5,165,952 A	11/1992	Solomon et al.	5,863,745 A	1/1999	Fitzgerald et al.
5,171,217 A	12/1992	March et al.	5,873,904 A	2/1999	Ragheb et al.
5,176,626 A	1/1993	Soehendra et al.	5,886,026 A	3/1999	Hunter et al.
5,182,317 A	1/1993	Winters et al.	5,893,867 A	4/1999	Bagaoisan et al.
5,197,977 A	3/1993	Hoffman et al.	5,902,283 A	5/1999	Darouiche et al.
5,217,493 A	6/1993	Raad et al.	5,916,596 A	6/1999	Desai et al. .... 424/489
5,222,971 A	6/1993	Willard et al.	5,921,952 A	7/1999	Desmond et al.
5,229,172 A	7/1993	Cahalan et al.	5,922,754 A	7/1999	Burchett et al.
5,232,685 A	8/1993	Speck et al.	5,954,706 A	9/1999	Sahatjian
5,234,456 A	8/1993	Silvestrin	5,977,163 A	11/1999	Li et al.
5,244,654 A	9/1993	Narayanan	5,980,972 A	11/1999	Ding et al.
5,282,823 A	2/1994	Schwartz et al.	5,981,568 A	11/1999	Kunz et al.
5,288,711 A	2/1994	Mitchell et al.	5,997,162 A	12/1999	English et al.
5,298,255 A	3/1994	Sawamoto et al.	6,010,480 A	1/2000	Abele et al.
5,304,121 A	4/1994	Sahatjian	6,013,092 A	1/2000	Dehdashtian et al.
5,306,286 A	4/1994	Stack et al.	6,017,948 A	1/2000	Rubinfeld et al.
5,314,688 A	5/1994	Kauffman et al.	6,039,721 A	3/2000	Johnson et al.
5,320,634 A	6/1994	Vigil et al.	6,071,285 A	6/2000	Lashinski et al.
5,342,348 A	8/1994	Kaplan	6,096,070 A	8/2000	Ragheb et al.
5,344,411 A	9/1994	Domb et al.	6,123,923 A	9/2000	Unger et al.
5,344,444 A	9/1994	Glastra	6,146,358 A	11/2000	Rowe
5,345,933 A	9/1994	Peterson et al.	6,171,232 B1	1/2001	Papandreou et al.
5,348,873 A	9/1994	Matsunda et al.	6,177,061 B1	1/2001	Klaveness et al. .... 424/9.51
5,356,433 A	10/1994	Rowland et al.	6,203,487 B1	3/2001	Consigny et al.
5,370,614 A	12/1994	Amundson	6,203,551 B1	3/2001	Wu
5,380,299 A	1/1995	Fearnot et al.	6,207,133 B1	3/2001	Reszka et al.
5,383,927 A	1/1995	De Goicoechea et al.	6,214,333 B1	4/2001	Zoldhelyi et al.
5,383,928 A	1/1995	Scott et al.	6,221,467 B1	4/2001	Nazarova et al.
5,419,760 A	5/1995	Narciso, Jr.	6,231,615 B1	5/2001	Preissman et al.
5,443,458 A	8/1995	Eury	6,240,616 B1	6/2001	Yan
5,447,724 A	9/1995	Helmus et al.	6,248,100 B1	6/2001	de Toledo et al.
5,449,382 A	9/1995	Dayton et al.	6,064,624 A1	7/2001	Desmond et al.
5,454,886 A	10/1995	Burrell et al.	6,258,108 B1	7/2001	Lary
5,455,040 A	10/1995	Marchant	6,264,624 B1	7/2001	Desmond et al.
5,456,663 A	10/1995	Lemelson	6,273,908 B1	8/2001	Ndondo-Lay
5,457,113 A	10/1995	Cillinan et al.	6,273,913 B1	8/2001	Wright et al.
5,464,450 A	11/1995	Buscemi et al.	6,287,285 B1	9/2001	Michal et al.
5,464,650 A	11/1995	Berg et al.	6,299,604 B1	10/2001	Ragheb et al.
5,500,013 A	3/1996	Buscemi et al.	6,306,151 B1	10/2001	Lary et al.
5,504,102 A	4/1996	Agharkar et al.	6,306,166 B1	10/2001	Barry et al. .... 623/1.46
5,510,330 A	4/1996	Martin et al.	6,335,029 B1	1/2002	Kamath et al.
5,531,716 A	7/1996	Luzio et al.	6,355,058 B1	3/2002	Pacetti et al.
5,534,288 A	7/1996	Gruskin et al.	6,364,856 B1	4/2002	Ding et al. .... 604/103.02
5,554,181 A	9/1996	Das	6,369,039 B1	4/2002	Palasis et al.
5,554,182 A	9/1996	Dinh et al.	6,369,093 B1	4/2002	Elbe et al.
5,559,448 A	9/1996	Koenig	6,375,931 B2	4/2002	Ostensen
5,567,495 A	10/1996	Modak et al.	6,406,754 B2	6/2002	Chappa et al.
5,569,463 A	10/1996	Helmus et al.	6,419,692 B1	7/2002	Yang et al.
5,571,086 A	11/1996	Kaplan et al.	6,479,033 B1	11/2002	Reszka et al.
5,578,075 A	11/1996	Dayton	6,491,619 B1	12/2002	Trauthen et al.
5,605,896 A	2/1997	Leonardi et al.	6,491,938 B2	12/2002	Kunz et al.
5,607,463 A	3/1997	Schwartz et al.	6,495,979 B2	12/2002	Park et al.
			6,500,341 B2	12/2002	Wang et al.

## US 8,257,305 B2

Page 3

6,503,954 B1	1/2003	Bhat et al.	CA	2 345 697 AA	5/2000	
6,515,016 B2	2/2003	Hunter et al.	CN	I 224 622 A	8/1999	
6,544,223 B1	4/2003	Kokish et al.	DE	4225553	5/1994	
6,544,544 B2	4/2003	Hunter et al.	DE	4225553 C1	5/1994	
6,562,024 B2	5/2003	Alvarez de Toledo et al.	DE	4446694	12/1994	
6,575,888 B2	6/2003	Zamora et al.	DE	4334272	4/1995	
6,585,765 B1	7/2003	Hossainy et al.	DE	4341478 A1	6/1995	
6,599,275 B1	7/2003	Fischer et al.	DE	44 35 652	4/1996	
6,599,448 B1	7/2003	Ehrhard et al.	DE	195 14 104	11/1996	
6,599,928 B2	7/2003	Kunz et al.	DE	69119753	1/1997	
6,616,591 B1	9/2003	Teoh et al.	DE	69403966	2/1998	
6,616,650 B1	9/2003	Rowe	DE	19724796 A1	12/1998	
6,635,082 B1	10/2003	Hossainy et al.	DE	69925936	6/2000	
6,638,913 B1	10/2003	Speck et al.	DE	10115740	10/2002	
6,656,156 B2	12/2003	Yang et al.	DE	10244847.7	11/2002	
6,682,545 B1	1/2004	Kester et al.	DE	69925936	7/2005	
6,682,546 B2	1/2004	Amplatz	DE	20122736	8/2007	
6,695,811 B2	2/2004	Samson et al.	EP	I 118 325 B1	11/1986	
6,706,892 B1	3/2004	Ezrin et al.	EP	0357003	3/1990	
6,730,064 B2	5/2004	Ragheb et al.	EP	0470246	2/1992	
6,774,278 B1	8/2004	Ragheb et al.	EP	0 551 182	7/1993	
6,867,190 B2	3/2005	Carney et al.	EP	0706376	7/1993	
6,918,927 B2	7/2005	Bates et al.	EP	0578998	1/1994	
7,060,051 B2	6/2006	Palasis et al.	EP	0604022	6/1994	
7,179,251 B2	2/2007	Palasis	EP	0623354	11/1994	
7,419,683 B2	9/2008	Szebeni et al.	EP	673114	9/1995	
7,445,792 B2	11/2008	Toner et al.	EP	0681475	11/1995	
7,491,234 B2	2/2009	Palasis et al.	EP	0706376 A1	4/1996	
7,611,532 B2	11/2009	Bates et al.	EP	0717041	6/1996	
7,731,685 B2	6/2010	Bates et al.	EP	0747069	12/1996	
7,750,041 B2	7/2010	Speck et al.	EP	0797988	10/1997	
7,811,622 B2	10/2010	Bates et al.	EP	0975340	2/2000	
2001/0014717 A1	8/2001	Hossainy et al.	EP	0 551 182 B1	7/2000	
2001/0034363 A1	10/2001	Li et al.	EP	0829238 B1	9/2000	
2001/0037140 A1	11/2001	Gaudoin et al.	EP	1037605	9/2000	
2001/0044651 A1	11/2001	Steinke et al.	EP	1090637	4/2001	
2002/0013549 A1	1/2002	Zhong et al.	EP	I 140273 B1	10/2001	
2002/0032414 A1	3/2002	Ragheb et al.	EP	I 669 092	12/2001	
2002/0037358 A1	3/2002	Barry et al.	EP	1250166	10/2002	
2002/0098278 A1	7/2002	Bates et al.	EP	1407786	4/2004	
2002/0123505 A1	9/2002	Burke et al.	EP	1447098	8/2004	
2002/0193828 A1	12/2002	Griffin et al.	EP	1512398	3/2005	
2003/0007944 A1	1/2003	O'Halloran et al.	EP	1521603	4/2005	
2003/0028243 A1	2/2003	Bates et al.	EP	1536850	6/2005	
2003/0028244 A1	2/2003	Bates et al.	EP	1159974	12/2005	
2003/0036794 A1	2/2003	Ragheb et al.	EP	I 666 071 A1	6/2006	
2003/0059454 A1	3/2003	Barry et al.	EP	1666070	6/2006	
2003/0100600 A1	5/2003	Kinsella et al.	EP	1669091	6/2006	
2003/0195548 A1	10/2003	Kester	EP	I 372 737 B1	8/2006	
2004/0068241 A1	4/2004	Fischer	EP	1695697	8/2006	
2004/0073284 A1 *	4/2004	Bates et al. .... 623/1.11	EP	1695698	8/2006	
2004/0115228 A1	6/2004	Costa et al.	EP	1735042	12/2006	
2004/0224003 A1 *	11/2004	Schultz ..... 424/423	EP	1781209	5/2007	
2004/0243225 A1	12/2004	Ragheb et al.	EP	2092941	8/2009	
2005/0042295 A1	2/2005	Hunter et al.	EP	2092942	8/2009	
2005/0063926 A1	3/2005	Bathina et al.	EP	2098230	9/2009	
2005/0101522 A1	5/2005	Speck et al.	JP	06-63145	3/1994	
2005/0123605 A1	6/2005	Hunter et al.	JP	6 63145	3/1994	
2005/0222677 A1	10/2005	Bates et al.	JP	06-063145	3/1994	
2005/0250672 A9	11/2005	Speck et al.	JP	7500585	1/1995	
2005/0278021 A1	12/2005	Bates et al.	JP	7-328124	12/1995	
2006/0020243 A1	1/2006	Speck et al.	JP	07-328124	12/1995	
2006/0020331 A1	1/2006	Bates et al.	JP	7 328124	12/1995	
2007/0128118 A1	6/2007	Yu et al.	JP	10 509691	9/1998	
2008/0012034 A1	1/2008	Thielen et al.	JP	10509691	9/1998	
2008/0102033 A1	5/2008	Speck et al.	JP	11012160 A	1/1999	
2008/0102034 A1	5/2008	Speck et al.	JP	2000 507930	6/2000	
2008/0118544 A1	5/2008	Wang	JP	2000507930	6/2000	
2008/0102034 A1	5/2008	Speck et al.	JP	2001 508320	6/2001	
2008/0175887 A1	7/2008	Wang	JP	2002 536058	10/2002	
2008/0255508 A1	10/2008	Wang	JP	36371777	3/2005	
2008/0255509 A1	10/2008	Wang	WO	WO-90/13293	11/1990	
2008/0255510 A1	10/2008	Wang	WO	WO-90/13332	11/1990	
FOREIGN PATENT DOCUMENTS				WO	WO-91/12779	9/1991
CA	2 207 025	6/1996	WO	WO 92/11890 A1	7/1992	
CA	2207025 AA	6/1996	WO	WO-92/11896	7/1992	
CA	2 218 103	10/1996	WO	WO 92/11890	7/1992	
CA	2 345 729 AA	4/2000	WO	WO-92/12717	8/1992	
			WO	WO 92/15282	9/1992	

## US 8,257,305 B2

Page 4

WO	WO 9215282	9/1992
WO	WO 9220718 A2	11/1992
WO	WO-93/06792	4/1993
WO	WO 93/07875	4/1993
WO	WO-93/09762	5/1993
WO	WO-93/09765	5/1993
WO	WO-93/11120	6/1993
WO	WO-93/11668	6/1993
WO	WO 00/50105 A2	2/1994
WO	WO 94/07484	4/1994
WO	WO-94/07529	4/1994
WO	WO-94/16706	8/1994
WO	WO 94/23787 A1	10/1994
WO	WO-94/25020	11/1994
WO	WO-94/26291	11/1994
WO	WO 95/03036 A1	2/1995
WO	WO 95/03083	2/1995
WO	WO 95/03795	2/1995
WO	WO 95/15782 A1	6/1995
WO	WO 96/17629	6/1996
WO	WO-96 39949	6/1996
WO	WO 96/20718	7/1996
WO	WO 96/25176	8/1996
WO	WO 96/25282	8/1996
WO	WO 96/38183	12/1996
WO	WO 96/39949 A1	12/1996
WO	WO 96/39970 A1	12/1996
WO	WO-97/01327	1/1997
WO	WO 97/26862	1/1997
WO	WO 97/17098 A1	5/1997
WO	WO-97/31674	9/1997
WO	WO 97/33552	9/1997
WO	WO-97/33552	9/1997
WO	WO-97 33552	9/1997
WO	WO-97/41916	11/1997
WO	WO 98/11933 A1	3/1998
WO	WO 98/14174	4/1998
WO	WO 98/15282 A1	4/1998
WO	WO 98/24427	6/1998
WO	WO 98/25176 A1	6/1998
WO	WO 98/30249	7/1998
WO	WO-98 31415	7/1998
WO	WO 0006152	7/1998
WO	WO 98/36784	8/1998
WO	WO-99 08729	8/1998
WO	WO-98/43618	10/1998
WO	WO 98/47540 A1	10/1998
WO	WO 98/43618	10/1998
WO	WO-99/08729	2/1999
WO	WO-99/09729	2/1999
WO	WO 99/12577 A1	3/1999
WO	WO 99/13916 A2	3/1999
WO	WO 99/19004 A2	4/1999
WO	WO-99 25336	5/1999
WO	WO-99/30684	6/1999
WO	WO-00 21584	10/1999
WO	WO 99/55396	11/1999
WO	WO-99/59556	11/1999
WO	WO 99/62510	12/1999
WO	WO-00/00023	1/2000
WO	WO-00/00238	1/2000
WO	WO-00 45744	1/2000
WO	WO 00/10552	3/2000
WO	WO 00/21584 A1	4/2000
WO	WO-00 32238	6/2000
WO	WO 00/32238 A1	6/2000
WO	WO-00 32267	6/2000
WO	WO 00/32267	6/2000
WO	WO 00/44414 A1	8/2000
WO	WO 00/45744	8/2000
WO	WO-00 45744	8/2000
WO	WO-00/47197	8/2000
WO	WO 0044414	8/2000
WO	WO 0045744	8/2000
WO	WO-01/24866	4/2001
WO	WO 01/24866 A1	4/2001
WO	WO 01/49338 A1	7/2001
WO	WO-01/54748	8/2001
WO	WO-01 76525	10/2001

WO	WO 01/83016 A2	11/2001
WO	WO 02066092	8/2002
WO	WO-02 076509 A2	10/2002
WO	WO-02 076509 A2	10/2002
WO	WO 02/076509 A2	10/2002
WO	WO-03 022264	3/2003
WO	WO 03/026718 A1	4/2003
WO	WO-03/41686	5/2003
WO	WO 03/048166	6/2003
WO	WO2004/006976	1/2004
WO	WO-2004/022124	3/2004
WO	WO 2004/028582	4/2004
WO	WO 2004/028610 A2	4/2004
WO	WO-2005/089855	9/2005
WO	WO-2005 112570	12/2005
WO	WO-2006/023104	3/2006
WO	WO-2008/063576	5/2008
WO	WO-2009/051614	4/2009
WO	WO-2009/051615	4/2009
WO	WO-2009/051616	4/2009
WO	WO-2009/051618	4/2009

## OTHER PUBLICATIONS

File History of U.S. Appl. No. 60/395,434, filed Jul. 12, 2002.

File History of U.S. Appl. No. 60,244,446, filed Oct. 31, 2000.

Ran Kornowski et al., "Slow-Release Taxol Coated GRIT™ Stents Reduce Neointima Formation in a Porcine Coronary In-Stent Restenosis Model," 70<sup>th</sup> Scientific Sessions of the American Heart Association, Nov. 9-12, 1997.

Alan W. Heldman et al., "Paclitaxel Stent Coating Inhibits Neointimal Hyperplasia at 4 Weeks in a Porcine Model of Coronary Restenosis," *Circulation*, May 8, 2001, pp. 2289-2295.

Department of Health and Human Services Notice of Intramural Research Project, Oct. 1, 1993-Sep. 30, 1994; "Molecular Strategies to Treat Restenosis," 4 pp.

Department of Health and Human Services Notice of Intramural Research Project, Oct. 1, 1994-Sep. 30, 1995, "Local Delivery of Therapeutic Agents for the Prevention of Restenosis," 6 pp.

Teruo Inoue et al., "Comparison of Activation Process of Platelets and Neutrophils After Coronary Stent Implantation Versus Balloon Angioplasty for Stable Angina Pectoris," *The American Journal of Cardiology*, vol. 86, Nov. 15, 2000, pp. 1057-1062.

Eric K. Rowinsky et al., "Paclitaxel (Taxol)", Alastair J.J. Wood, ed. "Drug Therapy," *The New England Journal of Medicine*, vol. 332, No. 15, Apr. 13, 1995, pp. 1004-1014.

Dorothea I. Axel et al., "Paclitaxel Inhibits Arterial Smooth Muscle Cell Proliferation and Migration in Vitro and in Vivo Using Local Drug Delivery," *Circulation*, 1997, vol. 96, pp. 636-645.

Bruno Scheller et al., "Acute Cardiac Tolerance of Current Contrast Media and the New Taxane Protaxel Using Iopromide as Carrier During Porcine Coronary Angiography and Stenting," *Investigative Radiology*, vol. 37, No. 1, pp. 29-34.

Martin Oberhoff et al., "Local delivery of Paclitaxel using the double-balloon perfusion catheter before stenting in the porcine coronary artery," 2001, *Catheterization and Cardiovascular Interventions*, pp. 562-568, vol. 53.

Christopher J. Creel et al., "Arterial Paclitaxel distribution and deposition," *Circulation Research*, Apr. 28, 2000, pp. 879-884.

Dr. Karsch, "Lokale Applikation von Paclitaxel mit dem Schneider-Doppelballon," nach experimenteller Stentimplantation an den Koronararterien des Schweines, Gießen 2001.

Toru Kataoka et al., "7-Hexanoyltaxol-Eluting Stent for prevention of Neointimal Growth," *Circulation*, Oct. 1, 2002, pp. 1788-1793.

Roger Charles et al., "Ceramide-coated balloon catheters limit neointimal hyperplasia after stretch injury in carotid arteries," *Circulation Research*, Aug. 18, 2000, pp. 282-288.

Elsevier Science Publishers, Amsterdam, NL; Jackson D.M. A. et al Current usage of contrast agents, anticoagulant and antiplatelet drugs in angiography and angioplasty in the UK. retrieved from STN Database accession No. 95327068 XP002226116.

International Preliminary Examination Report for PCT/DE2003/002871.

International Preliminary Examination Report for PCT/DE2001/04782.

## US 8,257,305 B2

Page 5

- Nishio, K., et al., "Enhanced Interaction Between Tubulin and Microtubule-Associated Protein 2 Via Inhibition of Map Kinase and CDC2 Kinase by Paclitaxel," *Int. J. Cancer*: 63, 688-693 (1995).
- Ding, A., et al., "Association of Mitogen-Activated Protein Kinases with Microtubules in Mouse Macrophages," *J. Exp. Med.*, vol. 183, Apr. 1996, 1899-1904.
- Lieu, C.-H., et al., "Role of Mitogen-Activated Protein Kinase in Taxol-Induced Apoptosis in Human Leukemic U937 Cells<sup>1</sup>," *Cell Growth & Differentiation*, vol. 9, pp. 767-776, Sep. 1998.
- Japanese Final Rejection in Co-pending Application No. JP2004-538964 dated Mar. 9, 2010.
- Opposition to corresponding EPI539266 by Boston Scientific Ltd., Mar. 10, 2010.
- Liggins, Richard T. et al., "Paclitaxel loaded poly(L-lactic acid) microspheres: properties of microspheres made with low molecular weight polymers," *International Journal of Pharmaceutics*, 2001, vol. 222, pp. 19-33.
- Dordunoo, S. K. et al., "Release of taxol from poly( $\epsilon$ -caprolactone) pastes: effect of water-soluble additives," *Journal of Controlled Release*, 1997, vol. 44, pp. 87-94.
- Wichert, B. et al., "Low Molecular weight PLA: a suitable polymer for pulmonary administered microparticles?" *J. Microencapsulation*, 1993, vol. 10, No. 2, pp. 195-207.
- Nairn, John A., "Polymer Characterization," *Materials Science & Engineering* 5473, 2003, Ch. 3, pp. 43-55.
- Cremers et al., "V1742—Paclitaxel-beschichtete PTCA-Katheter: Gibt es Unterschiede? Einfluss von PACCOATH und DIOR Balloinkathetern auf die Neointimnaproliferation an Schweinekronarien," *Clin. Res. Cardiol.*, 1997.
- Cremers, B. et al., "Comparison of two different paclitaxel-coated balloon catheters in the porcine coronary restenosis model," *Clin. Res. Cardiol.*, 2009, vol. 98, pp. 325-330.
- Grossmann, S., "Neuartige Zubereitungen Hemmung der Neointimnaproliferation in verengten Arterien," *Dissertation zur Erlangung des akademischen Grades des Doktors der Naturwissenschaften (Dr. rer. nat.)*, Nov. 2006.
- Sollott, Steven J. et al., "Taxol Inhibits Neointimal Smooth Muscle Cell accumulation after angioplasty in the rat," *The Journal of clinical Investigation*, Apr. 1995, vol. 95, pp. 1869-1876.
- BC, "Lippold in Retardarzneiformen" in E. Nurnberg, *Hagers Handbuch der pharmazeutischen Praxis*, vol. 2, Springer-Verlag Berlin Heidelberg New York, 5<sup>th</sup> edition, 1991, pp. 832-840.
- Langer, R., "New methods of drug delivery," *Science*, Sep. 28, 1990, vol. 249, pp. 1527-1533.
- Kirk-Othmer, *Encyclopedia of Chemical Technology*, 3<sup>rd</sup> Edition, vol. 17, 1982, John Wiley & Sons, pp. 281-310.
- Voigt, R., *Lehrbuch der pharmazeutischen Technologie*, 5<sup>th</sup> edition, VEB Verlag Volk und Gesundheit Berlin, 1984, p. 689.
- Tawashi, R., "The dissolution rates of crystalline drugs," *J. Mond. Pharm.* 1968, vol. 4, No. 11, pp. 371-379.
- Coomber and Gotlieb, *Arteriosclerosis*, 1990, vol. 10, No. 2, pp. 215-222.
- Bartoli et al., *J. Microencapsulation*, 1990, vol. 7, No. 2, pp. 191-197.
- Garcia-Matinez et al., "Effects of taxol on endothelial cells of the developing semilunar heart valves in the chick embryo," *Acta Anat.*, 1988, vol. 133, pp. 282-288.
- Muller et al., *JACC*, 1990, vol. 17, No. 6, pp. 126B-131B.
- Slepian, in *textbook of interventional cardiology*, 1990, Section IV, Chapter 32, pp. 647-670.
- Single e-mail from SIGMA Chemical Company of Feb. 15, 2007 to Dr. Sollot confirming that from 1991—1993 the material was listed in their catalog as "Taxol," and that the name was changed in their catalog from "taxol" to "paclitaxel" in 1994.
- Hiatt et al., "Drug-eluting stents for the prevention of restenosis: in quest for the Holy Grail," *Catheterization and Cardiovascular Interventions*, 2002, vol. 55, pp. 409-417.
- Forth, W. et al., "Allgemeine und spezielle Pharmakologie und Toxikologie," 7 Auflage. Heidelberg: Spektrum Akademischer Verlag, 1996, Chapter, 1, 2, 3.
- Liggins, R. T. et al., *J. Pharma. Sci.*, 1997, vol. 86, pp. 1458-1463.
- Matthew, R. T. et al., *J. Med. Chem.*, 1992, vol. 35, pp. 141-151.
- Tarr, B. D. et al., *J. Parent Sci. Technol.*, 1987, vol. 41, pp. 31-33.
- Swindell, C.S. et al., *J. Med. Chem.*, 1991, vol. 34, pp. 1176-1184.
- Sharma, U. S. et al., *J. Pharma. Sci.*, 1995, vol. 84, pp. 1223-1230.
- Barath et al., *JACC*, 1989, vol. 13, No. 4, pp. 252A.
- Cox et al., *Coronary Artery Disease*, 1992, vol. 3, pp. 237-248.
- Voisard et al., *Coronary Artery Disease*, 1993, vol. 4, pp. 935-942.
- Untersuchungen in vitro and in vivo, *Zeitschrift für kardiologie*, Band 89, Heft 5, 2000, pp. 390-397.
- Printout from the website of Bayer HealthCare Pharmaceuticals, indicating that Ultravist has been commercially available since 1985.
- Mitchel et al., *Circulation*, Oct. 1994, vol. 90, pp. 1979-1988.
- Kandarpa et al., *J. Vasc. Inter. Radiol.*, Nov./ Dec. 1997, vol. 8, pp. 997-1004.
- Kandarpa et al., *J. Vasc. Inter. Radiol.*, May/ Jun. 1998, vol. 9, pp. 487-493.
- Baron et al., *Cardiovascular Research*, Jun. 2000, vol. 46, pp. 585-594.
- Office Action issued by the European Patent Office on Sep. 15, 2005.
- Claims enclosed with Office Action issued by European Patent Office on Sep. 15, 2005.
- Response filed on Jan. 13, 2006.
- The decision to revoke EPI140273 B1 (=D11EP) of Oct. 23, 2007.
- Clinical Cardiology Divergent Effects on Coronary Artery Disease: Abstract from 70<sup>th</sup> Scientific Session: *Circulation*, vol. 96, No. 8, Oct. 21, 2007.
- Khan, I. et al., *Drug Development and Industrial Pharmacy*, 2005, vol. 31, pp. 59-78.
- Buaay KK, "Balloon Catheter for Intravascular Dosing," *Patent Abstracts of Japan*, Publication Date: Mar. 8, 1994, English Abstract of JP06-063145.
- Terumo Corp., "Medicine dosing catheter," *Patent Abstracts of Japan*, Publication Date: Dec. 19, 1995, English Abstract of JP07-328124.
- International Program on Chemical Safety, *General Chemical Information Chart*.
- Speck, Ulrich—German Priority Document for file No. 101 15 740.1 filed on Mar. 26, 2001.
- Parker, Sybil P., "Micelle," *McGraw-Hill Encyclopedia of Chemistry—Second Edition*, 1992, pp. 638-639.
- Sangster, J. et al., *Octanol-Water Partition Coefficients: Fundamentals and Physical Chemistry*, 1997, vol. 2 of Wiley Series in Solution Chemistry, pp. 1-49.
- Online Extract From SIGMA-Aldrich Web Site Concerning Poly Vinyl Alcohol (Molecular Weight: MW 500) 2008.
- Online Extract From SIGMA-Aldrich Web Site Concerning Poly Vinyl Alcohol (Molecular Weight: MS 1700) 2008.
- Online Extract From MSDS Online Concerning Sucrose 2007.
- Online Extract From Polysciences, Inc. Web Site Concerning Poly Lactic Acid (Molecular Weight: MW 1600 to 2400) 2008.
- Online Extract From Polysciences, Inc Web Site Concerning Polyvinylpyrrolidone (Molecular Weight: MW 2500) 2008.
- Online Extract From Polysciences, Inc. Web Site Concerning Polycaprolactone (Molecular Weight: MW 2000) 2008.
- Online Extract From Polysciences, Inc Web Site Concerning Polycaprolactone (Molecular Weight: MW: 1250) 2008.
- Online Extract From SIGMA-Aldrich Web Site Concerning Poly Acrylic Acid (Molecular Weight: MW 1800) 2008.
- Schwartz et al.: "Preclinical Restenosis Models and Drug-Eluting Stents", *Journal of the American College of Cardiology*, 2004, vol. 44, No. 7, p. 1373-1385, Elsevier Inc.
- Badapulle et al.: "A Hierarchical Bayesian Meta-Analysis of Randomised Clinical Trials of Drug-Eluting Stents", *Lancet*, 2004, vol. 364, pp. 583-591.
- Scheller et al.: "Treatment of Coronary In-Stent Restenosis With a Paclitaxel-Coated Balloon Catheter", *The New England Journal of Medicine*, 2006, vol. 355, No. 20, pp. 2113-2124.
- Licha et al.: "Hydrophilic Cyanine Dyes As Contrast Agents for Near-Infrared Tumor Imaging: Synthesis, Photophysical Properties and Spectroscopic in Vivo Characterization", *Photochemistry and Photobiology*, 2000, vol. 72, No. 3, pp. 392-398.
- Phillips et al.: "A-Level Biology", Oxford University Press, 1989, pp. 7-8.
- Pschyrembel *Klinisches Wörterbuch -German Clinical Dictionary and Reference Book* by Walter de Gruyter GmbH & Co. KG 1997, p. 717 (Hyperplasia).
- "Stent", [www.thefreedictionary.com/stent](http://www.thefreedictionary.com/stent), 2000.

## US 8,257,305 B2

Page 6

- "The Definition of Coated Stent", [www.medterms.com](http://www.medterms.com). 2003.
- "Balloon Catheter", [en.wikipedia.org/wiki/balloon\\_catheter](http://en.wikipedia.org/wiki/balloon_catheter), 2008.
- Singla, Ak et al.: "Paclitaxel and Its Formulations", *Int. J. Pharmaceutics* 235 (2002): 179-192.
- Nuijen, B. et al.: "Progress in the Development of Alternative . . ." *Investigational New Drugs*, 19 (2001): 143-153.
- Speck et al., *Inhibition of Restenosis in Stented Porcine Coronary . . .*, *Invest. Radiol.* 2004, 39, 182-186.
- Heartwire, Jan. 22, 2003: *Drug-eluting Stents: Where Are They Now?*, p. 2, Communication of [www.theheart.org](http://www.theheart.org).
- Scheller et al., *Addition of Paclitaxel to Contrast Media Prevents Restenosis After Coronary Stent Implantation*, *J. Am. Coll. Radiol.* 2003; 42:1415-1420.
- Scheller et al., *Paclitaxel Balloon Coating—A Novel Method for Prevention and Therapy of Restenosis*, *Circulation* 2004; 110:810-814.
- Li et al., *J. Nucl. Med.*, 38 (7), 1042-47 (1997).
- Perfluorocarbon Compounds As X-Ray Contrast Media in the Lungs *Bulletin Soc. Int. Chic.* 1975, 34 (2) 137-41.
- Paclitaxel: Ein Chemotherapeuticum Zur Restenoseprophylaxe? *Experimentelle Untersuchungen in Vitro Und in Vivo*, *Zeitschrift Fur Kardiologie*, Band 89, HEFT 5 (2000), pp. 390-397.
- Herdeg et al., *J. Am. Coll. Cardiol.* 35 1969-1976.
- Engelmann et al., 2007 *International Journal of Pharmaceutics* 329, 12-18.
- Print-out from an online tool for calculating a coefficient of distribution between octanol and water.
- Werk et al., "Inhibition of Restenosis in Femoropopliteal Arteries; Paclitaxel-Coated Versus Uncoated Catheter ; Femoral Paclitaxel Randomized Pilot Trial", *Circulation: Journal of the American Heart Association*, 2008, vol. 118, pp. 1358.
- Tepe et al., "Local Delivery of Paclitaxel to Inhibit Restenosis During Angioplasty of the Leg", *The New England Journal of Medicine*, 2008, vol. 358, No. 7, pp. 689-699.
- Henry et al., "'POBA Plus': Will the Balloon Regain Its Luster?", *Circulation: Journal of the American Heart Association*, 2008, vol. 118, pp. 1309-1311.
- Final Rejection dated May 1, 2008 in related U.S. Appl. No. 10/528,577, filed Mar. 21, 2005.
- Non-Final Rejection dated Jul. 2, 2007 in related U.S. Appl. No. 10/472,844, filed Sep. 26, 2003.
- Final Rejection dated Nov. 1, 2007 in related U.S. Appl. No. 10/472,844, filed Sep. 26, 2003.
- Non-Final Rejection dated May 29, 2008 in related U.S. Appl. No. 10/472,844, filed Sep. 26, 2003.
- Final Rejection dated Mar. 4, 2009 in related U.S. Appl. No. 10/472,844, filed Sep. 26, 2003.
- Non-Final Rejection dated Jan. 15, 2009 in related U.S. Appl. No. 10/618,977, filed Jul. 14, 2003.
- Non-Final Rejection dated Apr. 20, 2007 in related U.S. Appl. No. 10/618,977, filed Jul. 14, 2003.
- Baumbach et al., "Local Drug Delivery: Impact of Pressure, Substance Characteristics and Stenting on Drug Transfers into the Arterial Wall," *Catheterization and Cardiovascular Interventions*, Wiley-Liss, Inc., 1999, vol. 47, pp. 102-106.
- Series of extracts from the UK Trademarks Register, Apr. 29, 2008.
- IUPAC, *Compendium of Chemical Terminology* (1987).
- Table of General Chemical Information, Oct. 12, 2009.
- Product information DIOR balloon catheter of Eurocor GmbH, Oct. 1, 2008.
- Kalbitz et al., "Modulation der Wirkstoffpenetration in die Haut," *Pharmazie*, 1996, vol. 51, pp. 619-637.
- P. Macke Consigny et al., "Local Delivery of an antiproliferative drug with use of hydrogel-coated angioplasty balloons," *J. Vasc. Interv. Radiol.*, 1994, vol. 5, pp. 553-560.
- Drachmann et al., "Neointimal thickening after stent delivery of paclitaxel: Change in composition and arrest of growth over six months," *J. Am. Coll. Cardiol.*, 2000, vol. 36, pp. 2325-2332.
- Abstracts From the 70<sup>th</sup> Scientific Sessions, *Circulation*, Oct. 21, 1997, 96 Suppl. 1: 1-288.
- Van Belle, E. et al., "Passivation of metallic stents after arterial gene transfer of phVEGF165 inhibits thrombus formation and intimal thickening," *J. Am. Coll. Cardiol.*, 1997, vol. 29, pp. 1371-1379.
- Versuchsbeschreibungen (D44) ("Description of experiments"), Jul. 9, 2010.
- Affidavit (D46), Jul. 9, 2010.
- Final Report Study ACL435-43 (D47), May 14, 2009.
- Summary Data Biotronik SE & Co. KG (D48), Jul. 9, 2010.
- Submission BpatG (Ceramide Balloon Catheter) MLA HLA (D49), Jul. 9, 2010.
- German Translation of Gericht zu's Gravenhage, 245392/HA ZA May 2016 (D49A).
- Press release of Jan. 17, 2007 regarding patent infringement suit (D49C).
- Mortimer, C. et al., *Basiswissen Chemie* (excerpt) (1987) (D50).
- Summons to attend Oral Proceedings dated Jun. 4, 2010 (D51).
- Gershlick et al., "Inhibition of Restenosis with a Paclitaxel-Eluting, Polymer-Free Coronary Stent: The European evaluation of paclitaxel Eluting Stent (ELUTES) Trial," *Circulation*, 2004, vol. 109, pp. 487-493.
- Indolfi et al., "Smooth Muscle Cell Proliferation Is Proportional to the Degree of Balloon Injury in a Rat Model of Angioplasty," *Circulation*, 1995, vol. 92, pp. 1230-1235.
- Manderson et al., "Balloon Catheter Injury to Rabbit Carotid Artery. I. Changes in smooth muscle phenotype," *Arteriosclerosis*, 1989, vol. 9, pp. 289.
- Data Supplement to R. Charles et al., *Circulation Research*, 2000, vol. 87, pp. 282.
- Stemberger, Axel Dr., "Coating for bio-material to be used e.g. as sutures," Retrieved from Espacenet on Nov. 19, 2010; English Abstract of DE 4435652.
- Stemberger, Axel, Dr., "Coating for bio-material insertable into the bloodstream or tissue of the human body," Retrieved from Espacenet on Nov. 19, 2010; English Abstract of DE 19514104.
- Stemberger, Axel, Dr., "High efficiency local drug delivery," Retrieved from Espacenet on Nov. 19, 2010; English Abstract of DE 69925936.
- Morris, R. E. et al., "Method of treating hyperproliferative vascular disease using rapamycin, eventually in combination with mycophenolic acid," Retrieved from Espacenet on Nov. 19, 2010; English Abstract of EP0551182.
- Kaufmann, G. et al., "Process for producing a plastic cladding component and cladding component produced especially by said process," Retrieved from Espacenet on Nov. 19, 2010; English Abstract of WO9625282.
- Notice of Opposition to a European Patent. Patent No. 1 539 266 B1 filed by Fish & Richardson on behalf of Boston Scientific Limited. Received in the EPO on Jul. 29, 2008 (49 pages).
- Notice of Opposition. Objection to European Patent EU Patent 1 539 266 B1 filed by Karin Lindner-Vogt, European Patent Attorney on behalf of Opponent Biotronik VI Patent AG. English language (40 pages) and German languages (40 pages). Received in the EPO on Dec. 12, 2008. (Total pages 80).
- Evidence and Arguments in support of the grounds for opposition. Filed by Jacobacci & Partner on behalf of Opponent Invatec S.p.A. Proprietor: Bayer Schering Pharma Aktiengesellschaft. In re: Opposition against EP-B-1 539 266. Received in the EPO on Jan. 19, 2009. (7 pages).
- Notice and Statement of Grounds of Opposition against EP 1 539 266 filed by Williams Powell on behalf of Opponent Cook Incorporated. Date: Jan. 8, 2009. (33 pages).
- Opposition against EP 1 539 266 filed by Hoffmann-Eitle on behalf of Peter Klusman Jan. 9, 2009. (7 pages).
- Formal objection against EP Patent EP 1 539 266 B1 filed by ABK Patent, Trademark and Designs Attorneys on behalf of Eurocor GmbH. Date: Jan. 6, 2009. In the German language. (45 pages).
- Formal objection against EP Patent EP 1 539 266 B1 filed by ABK Patent, Trademark and Designs Attorneys on behalf of Eurocor GmbH. Date: Jan. 6, 2009. In the English language. (45 pages).
- Reply to the Notices by Bayer Schering Pharma AG. Main Request and as Auxiliary Request I through IV. In the English language. Date: Nov. 23, 2009. (18 pages).
- Reply by Bayer Schering Pharma AG. Main Request, Auxiliary Request II, III and IV. In the English language. Date: Nov. 23, 2009. (22 pages).

## US 8,257,305 B2

Page 7

Reply to the Notices filed by Weickmann & Weickmann on behalf of the Proprietor Bayer Schering Pharma AG. Date: Nov. 23, 2009. In the German language. (37 pages).

Documents submitted in view of the new Auxiliary Requests filed by Fish & Richardson on behalf of Boston Scientific Limited. Date: Mar. 10, 2010. (33 pages).

Summons to oral proceedings in compliance with Rule 115(1) European Patent Convention EPC issued by the EPO with comments to help parties to systematically prepare for the proceedings. Dated Sep. 1, 2010. Application No./Patent No. 03750300.0/1521/1539266. In the languages of English and German. (46 pages).

A pleading for the oral hearing on Feb. 16, 2011 submitted to the EPO filed by ABK Patent, Trademark and Designs Attorneys on behalf of Eurocor GmbH. Dated: Jan. 6, 2011. Re: New Documents Filed. In the language of English. (4 pages).

A pleading for the oral hearing on Feb. 16, 2011 submitted to the EPO by ABK Patent, Trademark and Designs Attorneys on behalf of Eurocor GmbH. Dated: Jan. 6, 2011. Re: New Documents Filed. In the language of German. EP Patent No. 1539266 B1. (4 pages).

Admissibility of the claims of the patent owner submitted to the EPO by ABK Patent, Trademark and Designs Attorneys on behalf of Eurocor GmbH. Dated: Jan. 4, 2011. EP Patent No. 1539266 B1. In language of English. (12 pages).

Admissibility of the claims of the patent owner submitted to the EPO by ABK Patent, Trademark and Designs Attorneys on behalf of Eurocor GmbH. Dated: Jan. 4, 2011. EP Patent No. 1539266 B1. In the language of German. (12 pages).

A pleading for the oral hearing on Feb. 16, 2011 submitted to the EPO according to Rule 115 (1) EPC by ABK Patent, Trademark and Designs Attorney on behalf of Eurocor GmbH. Dated: Jan. 4, 2011. In the language of English. EP Patent No. 1539266 B1. (4 pages).

A pleading for the oral hearing on Feb. 16, 2011 submitted to the EPO according to Rule 115 (1) EPC by ABK Patent, Trademark and Designs Attorney on behalf of Eurocor GmbH. Dated: Jan. 4, 2011. In the language of German. EP Patent No. 1539266 B1. (4 pages).

A submission for the oral hearing on Feb. 16, 2011 provided to the EPO according to Rule 115 (1) EPC by ABK Patent, Trademark and Designs Attorney on behalf of Eurocor GmbH. Dated: Jan. 4, 2011. In the language of English. EP Patent No. 1539266 B1. (20 pages).

A submission for the oral hearing on Feb. 16, 2011 provided to the EPO according to Rule 115 (1) EPC by ABK Patent, Trademark and Designs Attorney on behalf of Eurocor GmbH. Dated: Jan. 4, 2011. In the language of German. EP Patent No. 1539266 B1. (20 pages).

A further pleading for the oral hearing on Feb. 16, 2011 submitted to the EPO by ABK Patent, Trademark and Designs Attorney on behalf of Eurocor GmbH. Dated: Jan. 4, 2011. In the language of English. EP Patent No. 1539266 B1. (4 pages).

A further pleading for the oral hearing on Feb. 16, 2011 submitted to the EPO by ABK Patent, Trademark and Designs Attorney on behalf of Eurocor GmbH. Dated: Jan. 4, 2011. In the language of German. EP Patent No. 1539266 B1. (4 pages).

Newly submitted documents. Data Supplement to the scientific publication D4'n submitted to the EPO by ABK Patent, Trademark and Designs Attorney on behalf of Eurocor GmbH. Dated: Jan. 6, 2011. In the language of English. EP Patent No. 1539266 B1. (8 pages).

Newly submitted documents. Data Supplement to the scientific publication D4'n submitted to the EPO by ABK Patent, Trademark and Designs Attorney on behalf of Eurocor GmbH. Dated: Jan. 6, 2011. In the language of German. EP Patent No. 1539266 B1. (8 pages).

Correspondence dated Jan. 7, 2011. Submitted to the EPO by ABK Patent, Trademark and Designs Attorney on behalf of Eurocor GmbH. Re: Updated list of documents cited in the proceedings. In the languages of English and German. EP Patent No. 1539266 B1. (2 pages).

Further submissions for the hearing before the Opposition Division of the EPO. Re: Submitted documents. Submitted to the EPO by ABK Patent, Trademark and Designs Attorney on behalf of Eurocor GmbH. Re: Updated list of documents cited in the proceedings. In the languages of English and German. EP Patent No. 1539266 B1. Dated Jan. 12, 2011. (10 pages).

Submission by Bayer Schering Pharma. Claims modified in compliance with the main request and the auxiliary request I-IX supplied on the ruling dated Oct. 5, 2010. Exhibits, Main Request and auxiliary request I-IX. (pp. 78).

Submission by Bayer Schering Pharma. Claims modified in compliance with the main request and the auxiliary request I-IX supplied on the ruling dated Oct. 5, 2010. (38 pages).

A further submission for the hearing before the Opposition Division of the EPO on Feb. 14, 2011. Submitted to the EPO on Jan. 14, 2011 by ABK Patent, Trademark and Designs Attorney on behalf of Eurocor GmbH. Re: Updated list of documents cited in the proceedings. In the language of English. EP Patent No. 1539266 B1. (16 pages).

A further submission for the hearing before the Opposition Division of the EPO on Feb. 14, 2011. Submitted to the EPO on Jan. 14, 2011 by ABK Patent, Trademark and Designs Attorney on behalf of Eurocor GmbH. Re: Updated list of documents cited in the proceedings. In the language of German. EP Patent No. 1539266 B1. (6 pages).

Submission to the EPO by August & Debouzy Avocats on behalf of Invatek S.p.A. Dated Jan. 14, 2011. (2 pages).

Submissions in preparation for oral proceedings of Feb. 16, 2011. Submitted to the EPO by Williams Powell on behalf of Opponent IV Cook Inc. Dated: Jan. 14, 2011. (5 pages).

Submissions in preparation for oral proceedings of Feb. 16, 2011. Submitted to the EPO by Williams Powell on behalf of Opponent IV Cook Inc. Dated: Jan. 31, 2011. (6 pages).

Communication from the Examining Division of the European Patent Office issued on Sep. 15, 2005 in EP Application No. 03 750 300.0/1219. EP Patent No. 1539266.

Annex to the Communication from the Examining Division of the European Patent Office issued on Sep. 15, 2005 in EP Application No. 03 750 300.0/1219. EP Patent No. 1539266.

Reply and claims filed Jan. 13, 2006 in response to the Communication from the European Patent Office dated Sep. 15, 2005 in EP Application No. 03 750 300.0-1219. EP Patent No. 1539266.

English Translation of DE4225553 C1, 2011.

Atkins, Peter, "Chapter 7: Simple Mixtures," Physical Chemistry, 6<sup>th</sup> ed., 1997, pp. 176-186.

Leo, Albert et al., "Partition Coefficients and Their Uses," Chemical Reviews, Dec. 1971, vol. 71, No. 6, pp. 525-616.

Ulicky, L. et al., "Nernst's Distribution Law," Comprehensive Dictionary of Physical Chemistry, pp. 266-267, 1987.

Yushmanov, Victor E. et al., "Dipyridamole Interacts with the Polar Part of Cationic Reversed Micelles in Chloroform: <sup>1</sup>H NMR and ESR Evidence," Journal of Colloid and Interface Science, 1997, vol. 191, pp. 384-390.

Gold, Victor et al., "Amount of Substance Concentration," Compendium of Chemical Technology: International Union of Pure and Applied Chemistry Recommendations, 1987, p. 19.

Frank D. Kolodgie et al., Local delivery of ceramide for restenosis: Is there a future for lipid therapy? Circulation Research, Aug. 18, 2000, pp. 264-267.

Johnathan D. Adams et al., "Taxol: a history of pharmaceutical development and current pharmaceutical concerns," Journal of the National Cancer Institute Monographs, 1993, pp. 141-147, No. 15.

Jackson et al., "Current usage of contrast agents, anticoagulant and antiplatelet drugs in angiography and angioplasty in the UK," Clinical Radiology, 1995, pp. 699-704, vol. 50, No. 10.

Elsevier Science Publishers, Amsterdam, NL; Jackson D.M. A. et al

Current usage of contrast agents, anticoagulant and antiplatelet drugs

in angiography and angioplasty in the UK. retrieved from STN

Database accession No. 95327068 XP00226116, 1995.

International Preliminary Examination Report for PCT/DE2003/

002871, 2004.

International Preliminary Examination Report for PCT/DE2001/

04782, Jun. 24, 2003.

International Search Report for EP 06 00 1041, Search Date: Apr. 11,

2006.

International Search Report for EP 06 00 1042, Search Date: Apr. 10,

2006.

International Search Report for EP 06 00 1040, Search Date: Apr. 11,

2006.



## US 8,257,305 B2

Page 8


- International Search Report for PCT/DE01/04782, Search Date: Dec. 27, 2002.
- International Search Report for PCT/EP03/10480, Search Date: Feb. 20, 2004.
- International Search Report for PCT/DE03/02871, Search Date: Feb. 17, 2004.
- Brunner, H. et al., "Synthesis and in vitro testing of hematoporphyrin type ligands in platinum (II) complexes as potent cytostatic and phototoxic antitumor agents," *Inorganica Chimica Acta*, 1997, vol. 264, pp. 67-79.
- Bult, H., "Restenosis: a challenge for pharmacology," *TIPS*, Jul. 2000, vol. 21, pp. 274-279.
- Coomber, B. L. et al., "In vitro endothelial wound repair: Interaction of cell migration and proliferation," *Arteriosclerosis*, Mar. 1990, vol. 10, No. 2, pp. 215-222.
- Dichek, D. A. et al., "Seeding of Intravascular stents with genetically engineered endothelial cells," *Circulation*, 1989, vol. 80, No. 5, pp. 1347-1353.
- Elke M: *Kontrastmittel in der radiologischen Diagnostik*, pp. 113-119, 3<sup>rd</sup> edition, Georg Thieme Verlag Stuttgart New York, 1992.
- English Translation of Elke M: *Kontrastmittel in der radiologischen Diagnostik*, pp. 113-119, 3<sup>rd</sup> edition, Georg Thieme Verlag Stuttgart New York, 1992.
- Hamm, C. W. et al., "Guideline: Diagnostic Heart Catheter Examination," *Clin Res Cardiol*, 2008, vol. 97, pp. 475-512.
- English Translation of Hamm, C. W. et al., "Guideline: Diagnostic Heart Catheter Examination," *Clin Res Cardiol*, 2008, vol. 97, pp. 475-512.
- Hou, D. et al., "Intrapericardial paclitaxel delivery inhibits neointimal proliferation and promotes arterial enlargement after porcine coronary overstretch," *Circulation*, 2000, vol. 102, pp. 1575-1581.
- Khan, I. A. et al., "The Intra-vascular stent as a site-specific local drug delivery system," *Drug Development and Industrial Pharmacy*, 2005, vol. 31, pp. 59-78.
- Lamba, N. M. K. et al., *Polyurethanes in Biomedical Applications* Chapter 4, "Structure and Physical Characterization of Polyurethanes," 1998, CRC Press.
- Lübbe, A. S. et al., "Preclinical experiences with magnetic drug targeting: Tolerance and Efficacy," *Cancer Research*, 1996, vol. 56, pp. 4694-4701.
- Nicolaou, K. C. et al., "Design, synthesis and biological activity of protaxols," *Nature*, Jul. 29, 1993, vol. 364, pp. 464-466.
- Schmitz, S. A. et al., "Superparamagnetic iron oxide-enhanced MRI of atherosclerotic plaques in Watanabe Hereditary Hyperlipidemic Rabbits," *Investigative Radiology*, Aug. 2000, vol. 35, No. 8, pp. 460-471.
- English Abstract of JP-06 063145, "Balloon Catheter for intravascular dosing," Buayyu KK, Patent Abstracts of Japan, Publication Date: Mar. 8, 1994.
- English Abstract of JP-6 063145, "Balloon Catheter for Intravascular dosing," Buayyu KK, Thomson Innovation, Publication Date: Mar. 8, 1994.
- English Abstract of JP-07 328124, "Medicine dosing catheter," Terumo Corp., Patent Abstracts of Japan, Publication Date: Dec. 19, 1995.
- Patent Family Listing for JP-2001 508320 (Publication Date: Jun. 26, 2001), Thomson Innovation.
- Patent Family Listing for JP-2002 536058 (Publication Date: Oct. 29, 2002), Thomson Innovation.
- English translation of Decision of Final Rejection, Japanese Application No. 2004 235694, issued Mar. 9, 2010.
- English Translation of JP 36371777 (Publication Date: Mar. 23, 2005), Thomson Innovation.
- Submission by Eurocor, filed Feb. 18, 2011, in EPO Opposition against EP 1 539 266.
- English Translation of Submission by Eurocor, Feb. 18, 2011, in EPO Opposition against EP 1 539 266.
- Minutes of Oral Hearing, May 3, 2011, in Opposition against EP 1 539 266.
- English translation of Minutes of Oral Hearing, May 3, 2011, in Opposition against EP 1 539 266, issued May 3, 2011.
- EPO Decision to revoke EP 1 539 266, in EPO Opposition against EP 1 539 266.
- English Translation of Decision to revoke the EP Patent, in EPO Opposition against EP 1 539 266.
- Grounds of Appeal, filed Sep. 12, 2011, by Bayer Pharma AG, in EPO Opposition against EP 1 539 266 (with Main and Auxiliary Requests).
- English Translation of Grounds of Appeal, filed Sep. 12, 2011, by Bayer Pharma AG, in EPO Opposition against EP 1 539 266 (with Main and Auxiliary Requests).
- Response to Appeal, filed Oct. 13, 2011 by Boston Scientific, in EPO Opposition against EP 1 539 266.
- Response to Appeal, filed Jan. 20, 2012 by Cook Inc., in EPO Opposition against EP 1 539 266.
- Response to Appeal, filed Jan. 26, 2012 by Dr. Peter Klusmann, in EPO Opposition against EP 1 539 266.
- Cancellation Action against DE 203 21 606 filed in the German Patent Office by Eurocor (Sep. 6, 2010).
- English Translation of Cancellation Action against DE 203 21 606 filed in the German Patent Office by Eurocor (Sep. 6, 2010).
- Submission by Bayer Schering Pharma (BSP) filed Feb. 25, 2011 in Cancellation Action against DE 203 21 606.
- Thomson Innovation, Patent Record View, Publication Date: Sep. 22, 1998; English abstract of JP-10 509691.
- Thomson Innovation, Patent Record View, Publication Date: Jan. 19, 1995; English abstract of JP-7 500585.
- English Translation of Submission by Bayer Schering Pharma (BSP) filed Feb. 25, 2011 in Cancellation Action against DE 203 21 606.
- Submission by Eurocor filed Apr. 20, 2011 in Cancellation Action against DE 203 21 606.
- English Translation of Submission by Eurocor filed Apr. 20, 2011 in Cancellation Action against DE 203 21 606.
- Submission by Bayer Schering Pharma (BSP) filed Sep. 30, 2011 in Cancellation Action against DE 203 21 606.
- English Translation of Submission by Bayer Schering Pharma (BSP) filed Sep. 30, 2011 in Cancellation Action against DE 203 21 606.
- Submission by Eurocor filed Dec. 2, 2011 in Cancellation Action against DE 203 21 606.
- English Translation of Submission by Eurocor filed Dec. 2, 2011 in Cancellation Action against DE 203 21 606.
- Office Action issued Aug. 16, 2011 in U.S. Appl. No. 12/835,420.
- Office Action issued Oct. 13, 2011 in U.S. Appl. No. 11/763,116.
- Office Action issued Dec. 16, 2011 in U.S. Appl. No. 12/835,414.
- Office Action issued Feb. 16, 2012 in U.S. Appl. No. 12/782,989.
- Office Action issued Mar. 9, 2012 in U.S. Appl. No. 12/835,420.
- Judgment of Sep. 16, 2011 (Paper No. 52) from Interference No. 105,787.
- Redeclaration of Interference (Paper No. 48) issued Sep. 13, 2011.
- Applicants' Amendment of Sep. 12, 2011 (Paper No. 47), filed in U.S. Appl. No. 11/763,125, and cited in the Judgment of Sep. 16, 2011 in Interference No. 105,787.

\* cited by examiner

**U.S. Patent**

**Sep. 4, 2012**

**US 8,257,305 B2**

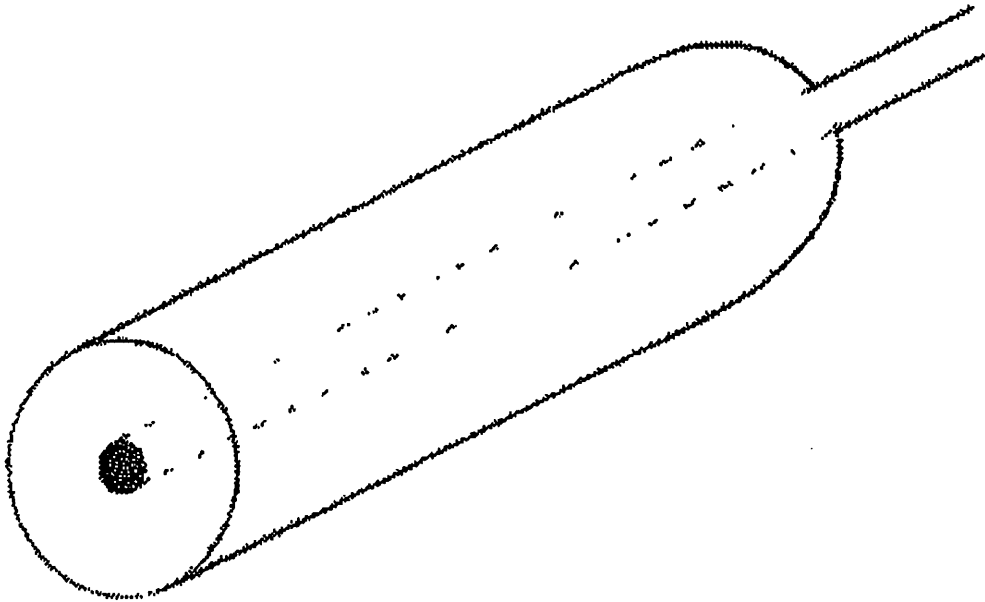

US 8,257,305 B2

1

# MEDICAL DEVICE FOR DISPENSING MEDICAMENTS

This invention relates to a medical apparatus that releases drugs for the selective therapy of specific tissues or organ parts and to a method of manufacturing such drug-coated devices.

Numerous diseases do not affect the entire organism at the same time but are restricted to specific tissues, often even to very limited individual tissue areas or organ parts. Examples can be found among tumor, joint and vascular diseases.

Pharmacotherapy of such diseases generally is effected by oral or intravenous administration of drugs that spread throughout the body and cause undesirable side effects in healthy tissues and organs, especially when the disease to be treated is in a severe stage, which limit the therapeutic application. The diseased tissues could be treated either selectively using drugs that specifically bind to diseased tissue (e.g. antibodies) while the administration path is maintained, or by selective administration, e.g. direct injection into the diseased tissue or supply via a catheter to the blood vessels that feed the diseased tissue. In case of selective administration may problems arise due to the short period of time during which the drugs are efficacious and the invasive administration paths, as repeated administration is not an option. When drugs are selectively administered via the bloodstream that feeds the diseased tissue, there is the additional problem that the drugs are insufficiently extracted when the blood or active agent solution swiftly flows through the blood vessels.

These problems used to be addressed by various pharmaceutical preparations with sustained release of the active agent, drug-releasing implants or selective access paths that stay operational for a longer period of time such as implanted catheters, etc.

It is known that the surface of medical equipment inserted into the body, in particular, of catheters, can be coated with agents that enhance gliding quality or prevent blood coagulation but have no therapeutic effect.

In addition, catheters are equipped with special devices for injecting drugs into the arterial wall, for example, using needles or a perforation of the catheter wall that sits adjacent to the vessel wall and through which the drug is injected at high pressure.

Other principles are based on extending the contact time between the arterial wall and an active agent preparation administered via the catheter by either blocking the blood flow for a sufficient period of time, e. g. using dual balloon catheters in which the active agent solution is contained in a chamber between the balloons, or by voids between a toric outer wall of the balloon allowing a limited flow of blood through a canal that passes through the balloon.

According to U.S. Pat. No. 5,102,402, drugs in the form of microcapsules are inserted into preformed recesses of balloon catheters for delayed release of the active agent. When the balloon is inflated, the microcapsules are to be pressed against the vessel wall, remain there and slowly release the active agent(s). Many authors propose to apply drugs embedded in hydrogel onto balloon catheters while they do not specify the function of the hydrogel, i. e. to act as an adhesive, to improve the gliding quality, or for controlled drug release.

A disadvantage of the products mentioned above is their complex structure, which causes production, quality control, and cost problems and forces additional aggravating working steps on doctors and patients when applied. Some of the methods mentioned may result in undesirable vascular damage in excess of the intended dilatation of the vessel. Another

2

setback is that each measure aimed at extending contact time entails another reduction in blood and oxygen supply to the downstream tissues.

For the sake of completeness, we also refer to a device for preventing restenosis as described in WO 01/24866 that is coated with a lipid ceramide substance derived from natural cell membranes. This substance is used because of its affinity to cell walls that is not found in common drugs. Experts in the field continue to state that restenosis prevention using drugs requires release of the active agent over a period of several days.

The problem underlying the present invention is to provide a device for the release of drugs into specific tissue areas or organ parts that has a strong therapeutic effect without damaging healthy tissue, which is sufficiently well tolerated, and can be produced and applied with a minimal effort.

This problem is solved according to the invention by a medical device that releases drugs for the selective therapy of specific diseased tissues or organ parts, characterized in that lipophilic, largely water-insoluble drugs that bind to any tissue components adhere to the surfaces of devices that come into contact with the diseased tissue by being pressed against it at least for a short time and immediately release the active agent when in contact with tissue, and of a method for producing such a device characterized in that the lipophilic drugs and excipients in a solution, suspension or emulsion medium are applied using an immersion, spreading, or spraying process or an instrument which delivers a defined volume to the surface of the device while excess media and substances that adhere loosely to the surface are removed.

The invention provides improved drug-carrying balloon catheters or similar medical devices manufactured in a simple process that are highly versatile and facilitate the immediate release of active agents. Surprisingly, and contrary to the currently acknowledged opinion, no continuing release of the active agent from an inert matrix (polymer, hydrogel, microcapsule, etc.) and no special chemical or physical state of the active ingredients is required or useful. Therefore, no sophisticated techniques for producing or controlling depot formulations are required.

Coating balloons on catheters with drugs according to this invention is particularly useful because there is a frequent need for treatment after blood vessels or other passages in the body were dilated with balloons to prevent stenosis or an occlusion of the lumen created by the pressure of the balloon, to limit tumor growth or to enhance healing processes including the formation of collateral circulation. This can be achieved by drugs that become effective in the immediate vicinity of the balloon surface. The drugs firmly adhere to the balloon while passing through arteries with an intense blood flow on their way to their target until the balloon is inflated, and an effective dose is released in the short time (sometimes just a few seconds) during which the inflated balloon is in contact with the tissue, absorbed by the tissue in such a way that the blood flow that resumes immediately after the balloon is deflated does not rinse it off.

The subjects for coating are wires of the invention used to guide catheters, needles and catheters or catheter parts that are pressed against the diseased tissue at least for a short time. Preferred catheter materials are polyamides, polyamide mixtures and copolymers, polyethylene terephthalate, polyethylene and copolymers, polyurethane, natural rubber and its derivatives. The lengths and diameters of the catheter or balloon areas designated for pharmacological treatment are not of any decisive importance for their application as the dosage is calculated in  $\mu\text{g}$  of active agent/ $\text{mm}^2$  of surface area. For example, balloons with diameters ranging from 2 to 4 mm and

US 8,257,305 B2

3

lengths ranging from 1.0 to 4.0 cm are commonly used for coronary dilatation. Balloons up to >20 mm in diameter and up to >10 cm in length can be used for other vessels. The surfaces to be coated may be smooth (i.e. without a special structure for absorbing the active agents), roughed up or comprise any structure; while no special surface structures are required for the active agents to adhere, such structures also do not impede adhesion. Adhesion of the active agents to the balloon surfaces is exclusively caused by selecting suitable solvents and, optionally, adding substances that influence adhesion. It is even surprisingly strong on completely smooth balloon surfaces.

All surfaces can additionally be coated with substances that improve the gliding quality of the products, prevent blood from coagulating on the surface or improve any other properties of these medical products have but the materials used for coating do not have to be released into the environment and this additional coating does not noticeably reduce the release of the active agents for treatment of the target tissue and thus the product's efficacy.

Balloon catheters are formed by dilating a segment of 1 cm to ca. 10 cm length of very thin plastic tubes. The dilated, very thin-walled balloon membrane is then folded several times along the catheter axis and wrapped tightly around the catheter axis so that the dilated area, when folded, is only slightly greater in diameter than the rest of the catheter. The tight folding of the balloon membrane is required for passing the balloon catheter through access ports, guiding catheters and heavily stenosed sections of blood vessels.

The balloons of catheters can be coated when folded or when unfolded. The process always provides an intact and sufficiently uniform surface coating, and the active agents adhere to the surface of the balloon catheter even when it is refolded after being coated when unfolded.

A balloon that was coated when unfolded is produced without any impact on the coating, for example by using balloon membranes with preformed folds and bends whose structure is not lost due to dilatation and which allow the balloon membrane to refold at least loosely when the pressure is discharged from the balloon without requiring an external force as primary cause. It is only after this preforming that the preformed folds are compressed by external pressure or by a vacuum. Folds are in no way required to hold the active agent. In addition refolding can be achieved using minor mechanical force by very smooth materials, and the tools used may also be wetted by slippery biocompatible liquids in which the active ingredients do not or, at least, do not well dissolve.

In accordance with another variant of the invention, the balloons of readily folded balloon catheters are coated by dipping them into low-viscosity active agent solutions. Solvent and active agent penetrate into the extremely dense folds where they form a surprisingly uniform coat that contains a reproducible dose and is not damaged by any subsequent step. The solution or, after the solvent has dried, the coat that adheres to the outer surface may be left there or may be removed in another step so that only the active agent portion that sits inside the folds of the balloon is retained.

After coating, when the balloon is folded, a stent can be pulled over the balloon catheter and firmly pressed onto it. The only step still required is sterilization, e.g. using ethylene oxide.

The work cycle laid out like this is extremely simple, hardly susceptible to failures, and can be carried out even with mechanically, chemically and physically sensitive coating materials. It was found that coating using this method does not result in any undesirable loosening or sticking together of the folds and that the active agent applied in this way adheres

4

firmly enough to not be rinsed off by the bloodstream but releases most of the active agent when the balloon is inflated in the target tissue.

Suitable drugs are lipophilic, mostly water-insoluble and strongly acting drugs that bind to any tissue components. Drugs are called lipophilic when their butanol to aqueous buffer solution (pH 7) distribution ratio is 0.5, preferably 1 and particularly preferred 5, or when their octanol to aqueous buffer solution (pH 7) distribution ratio is 1, preferably 10, and particularly preferred greater than 50. Alternatively, or in addition to this, the drugs should reversibly and/or irreversibly bond to cell components at percentages greater than 10%, preferably greater than 50%, and particularly preferred greater than 80%. Preferred are substances that inhibit cell proliferation or inflammatory processes, or antioxidants such as Paclitaxel and other taxanes, Rapamycin and related substances, tacrolimus and related substances, corticoids, sexual hormones (estrogen, estradiol, antiandrogens) and related substances, statins, epothilones, probucol, prostacyclins, angiogenesis inducers, etc.

These substances are preferably present as a dry solid or as an oil on the surfaces of the various medical products. Preferred are the smallest particle sizes (mostly <5 microns, preferably <1 microns, particularly preferred <0.1 microns), particularly preferred are amorphous non-crystalline structures of the finest particle size that dissolve fast upon contact with tissue due to their large surface area and despite the generally poor water-solubility of the drugs and do not function as microcapsules, i. e. dissolve spontaneously and fast. It is sufficient that an effective dose is present in the form of smallest or amorphous particles; larger particles hardly contribute to the active agent concentration in the tissue but do not cause any interference. The dosage depends on the desired effect and the efficacy of the drug used. It may be up to 5 µg/mm<sup>2</sup> and this value does not even constitute an upper limit. It is easier to handle smaller dosages.

Good adhesion to the surfaces of catheters, needles or wires on an improved absorption by the tissues is achieved by embedding strongly lipophilic active agents with poor water solubility in a readily water-soluble matrix substance. Suitable matrix substances are low-molecular (molecular weight <5000 D, preferably <2000 D) hydrophilic substances such as contrast agents and dyes used in vivo for various diagnostic procedures in medicine, sugar and related substances such as sugar alcohols, low-molecular polyethylene glycols, biocompatible organic and inorganic salts such as, for example, benzoates, salts and other derivatives of salicylic acid, etc. Examples of contrast agents are iodinated X-ray contrast agents and paramagnetic chelates, examples of dyes are indocyanine green, fluorescein, and methylene blue. Excipients may also improve shelf life of the products, cause specific additional pharmacological effects or be instrumental for quality control.

In another embodiment of the invention, the pharmaceutical active agents can be adsorbed to particles or applied to the surfaces of suitable medical products with a low-molecular matrix. Suitable particles once again are diagnostics known to be biocompatible such as ferrites and various contrast agents for sonography.

Excipients of any kind can be used at lower or higher doses than the active ingredients.

The medical products are coated using solutions, suspensions, or emulsions of the drugs and excipients mentioned above. Suitable media for solution, suspension or emulsion are, for example, ethanol, isopropanol, ethyl acetate, diethyl ether, acetone, dimethyl sulfoxide, dimethyl formamide, glycerin, water or mixtures thereof. Solvent selection is based

US 8,257,305 B2

5

on the solubility of the active agents and adjuvants, the wetting of the surfaces to be coated and the effect on the structure of the coating and particles remaining after evaporation of the solvent, their adhesion to the surface and active agent transfer to the tissue in very short contact times.

Coating can be carried out by immersing, spreading, applying with devices which deliver a defined volume to the surface or spraying at various temperatures and, optionally, vapor saturation of the solvents in the atmosphere. The procedure can be repeated several times using different solvents and excipients as may be required.

The balloons of folded balloon catheters ready for use can be given a surprisingly uniform, reproducible, dose-controllable coating without impairing catheter functionality by immersing them in solutions containing the active agent(s) or by other measures. When the balloons are repeatedly immersed in unsaturated active agent solutions, the active agent applied previously is not completely stripped off; instead, the active agent content of the balloons is increased in a reproducible manner.

Excess solution or excess substances from the coating solution that are loosely attached to the exterior can be removed with simple methods without impairing the efficacy of the coating.

The various types of medical devices designed and manufactured according to the invention come into short-term contact with the tissue, i. e. for a few seconds, minutes, or hours. It is desirable in some cases to pharmacologically treat the tissue with drugs in the immediate vicinity of the medical product, e. g. to prevent excess growth as a response to an injury or to reduce tumor growth, to enhance neovascularization or diminish inflammatory reactions. In all these cases, high local drug concentrations can be achieved for an astonishingly long time using the method described above. A major advantage is the extraordinary versatility of uses of the products and methods described.

A preferred application is to reduce hyperproliferation of vessel walls induced by dilatation with balloon catheters. This can be achieved when stents are implanted by coating these stents with drugs, but only for the vessel section covered by the stent. The coated balloon catheters also treat any areas at short distance in front of and just behind the stent that need treatment, they can treat the section where a stent has been implanted without requiring another stent implantation and vessels in which no stent is to be or can be implanted. An advantage as compared to the stents that release a drug over a long period of time is improved healing and simultaneous good inhibition of hyperproliferation and a reduced risk of thrombosis.

Several embodiments of the invention will be described below with reference to examples regarding the coating of balloon catheters, adhesion of the coating in the bloodstream, restenosis inhibition and active agent content of the catheters.

#### BRIEF DESCRIPTION OF THE DRAWING

FIG. 1 shows a catheter with an expanded balloon on which a coating of this invention can be applied.

#### EXAMPLE 1

Coating an Expanded Balloon Catheter with Paclitaxel in Ethyl Acetate

Balloon catheters made by BMT, Oberpfaffenhofen/Munich, Germany, product name Joker Lite, balloon dimensions 2.5 mm by 20 mm, are inflated to the maximum and immersed full length for 1 minute in ethyl acetate, 18.8 mg Paclitaxel per

6

ml, +1% pharmaceutical olive oil, dried: Paclitaxel content 39 micrograms (after extraction with ethanol, HPLC).

#### EXAMPLE 2

Coating a Folded Balloon Catheter with Paclitaxel in Ethyl Acetate

Balloon catheters made by BMT, Oberpfaffenhofen/Munich, Germany, product name Joker Lite, balloon dimensions 2.5 mm by 20 mm, are immersed full length in folded condition for 1 minute in ethyl acetate, 18.8 mg Paclitaxel per ml, +1% pharmaceutical olive oil, and dried: Paclitaxel content 69 micrograms.

#### EXAMPLE 3

Coating a Folded Balloon Catheter with Paclitaxel in Ethyl Acetate

a) Balloon catheters made by BMT, Oberpfaffenhofen/Munich, Germany, product name Joker Lite, balloon dimensions 2.5 mm by 20 mm, are immersed full length in folded condition for 1 minute in ethyl acetate, 16.6 mg Paclitaxel per ml, and dried for 4 hours: Paclitaxel content 54 micrograms.

b) Same procedure, but additional two times immersed for 5 seconds with 1 hour drying time after each immersion process in solution A (=3.33 ml ethyl acetate +100.0 mg of Paclitaxel): Paclitaxel content 126 micrograms.

c) Same procedure, but additional four times immersed for 5 seconds with 1 hour drying time after each immersion process in the same solution: Paclitaxel content 158 micrograms.

#### EXAMPLE 4

Coating a Balloon Catheter with Paclitaxel in Acetone

Dissolve 350 mg of Paclitaxel in 9.0 ml of acetone; balloon catheters made by BMT, Oberpfaffenhofen/Munich, Germany, product name Joker Lite, balloon dimensions 2.5 mm by 20 mm, are inflated to the maximum and immersed full length for 1 minute and removed. The solvent is dried for 12 hours at room temperature. Then the balloon is deflated and folded in the common way using a PTFE-coated tool. Optionally, one can crimp a stent of suitable dimensions onto the balloon: 29 micrograms of Paclitaxel on the balloon.

#### EXAMPLE 5

Coating a Balloon Catheter with Paclitaxel in Acetone

a) Immersion of folded balloon catheters made by BMT, product name Allegro, balloon dimensions 2.5 by 20 mm in a mixture of 0.15 ml ethanol +4.5  $\mu$ l of Ultravist 300 (an X-ray contrast agent made by Schering AG, Berlin, Germany) +1.35 ml of acetone +0.8 mg of Sudan red +30.0 mg of Paclitaxel: The folded balloon sections of the catheters are immersed 5 times, the first time for one minute, then dried for 3 hours, then 4 times at 1 hour intervals for 5 seconds each; subsequently, a stent was crimped on and the catheter was sterilized in the common way using ethylene oxide: Paclitaxel content 172 micrograms, no decomposition products of the active agent were determined using HPLC

b) A saturated aqueous mannitol solution is used instead of Ultravist 300

c) A saturated aqueous sodium salicylate solution (pH 7.5) is used instead of Ultravist 300

## US 8,257,305 B2

7

- d) 5 mg of acetylsalicylic acid are added to the completed solution according to (5a).  
 e) 5 mg of glycerin are added to the completed solution according to (5a).

## EXAMPLE 6

## Adhesion of the Active Agent in the Bloodstream

12 balloon catheters made by BMT, product name Allegro, balloon dimensions 2.5 by 20 mm, were used. The folded balloon sections of 6 catheters each were either 5 times immersed in [0.15 ml of ethanol +4.5 ul of Ultravist 300+1.35 ml of acetone +0.8 mg of Sudan red +30.0 mg Paclitaxel] or 5 times in [1.5 ml of ethyl acetate +0.8 mg Sudan red +31.0 mg Paclitaxel], the first time for 1 minute each with 3 hours of drying time, then 4 times for 5 seconds each at 1 hour intervals; then 3 of the folded balloons of each group were gently moved for 5 minutes at 37° C. in 50 ml of human blood and removed to determine the Paclitaxel content: Reduction of mean values (n=3 per coating method) by 5 minutes of movement in blood as compared to 3 control catheters that were not incubated in blood.

Acetone:	12%
Ethyl acetate:	10%

## EXAMPLE 7

## Examination of Restenosis Inhibition after Angioplasty and Stent Implantation in Coronary Arteries of Pigs.

Folded balloon catheters of the Joker Lite type made by BMT, 3.5 by 20 mm or 3.0 by 20 mm were immersed for 1 minute either in solution A) 3.33 ml of ethyl acetate (EA)+100.0 mg of Paclitaxel, or in solution B) 0.45 ml of ethanol +100 ul of Ultravist-370+4.5 ml acetone (ac) +150.0 mg Paclitaxel and dried over night at room temperature. One more (low dose=L) or 4 more (high dose=H) immersion process(es), respectively, were carried out for just five seconds at 1 hour intervals on the next day. Active agent content after 2 immersions in solution (B) averaged 250 µg, after 5 immersions in solution (B) 500 µg, in solution (A) 400 µg.

The catheters coated with Paclitaxel or uncoated were used to implant stents into the left anterior or lateral coronary artery of a total of 22 pigs, and the vessels were slightly overdilated to stimulate restenosis by tissue hyperplasia. The animals were reangiographed after 5 weeks, and the vessel stenosis shown in the angiograms was measured using an automatic computer program.

Group	Stenosis (%)
Uncoated	50.49
AcL	20.22
EAH	36.01
AcH	0.86
P	.004

Quantitative coronary angiography 5 weeks after stent implantation with uncoated and coated catheters; stenosis=reduction of lumen diameter in percent in the area of the stent as compared to the lumen diameter immediately

8

after stent implantation; mean value and statistical significance of the effect of treatment.

## EXAMPLE 8

## Active Agent Content of the Catheters after Vessel Dilatation and Stent Implantation

After stent implantation and removal from the animals, the balloons from Example 7 ca. 3 cm in length were cut off the balloon catheters and placed in 1.5 ml of ethanol. Paclitaxel content was determined using HPLC. All available coated balloons and a selection of uncoated balloons were examined.

## Coronary,

3.0 by 20 mm, coating:	Ac high	38 ± 4 µg (n = 4)
	Ac low	22 ± 5 µg (n = 2)
	EEE high	41 (n = 1)
3.5 by 20 mm, coating:	Ac high	37 ± 10 µg (n = 8)
	Ac low	26 ± 6 µg (n = 8)
	EEE high	53 ± 9 µg (n = 9)
Uncoated (independent of size and vessel area)		0.9 ± 1.0 µg (n = 7)

It follows from Example 6 that a maximum of 10% of the dose is lost before the balloon is inflated and about 10% of the dose remain on the balloon.

## EXAMPLE 9

Probucol is added to acetone at a concentration of 100 mg per ml; the solution is used to coat balloon catheters as described in the above examples.

## EXAMPLE 10

Rapamycin is dissolved at a concentration of 10 mg/ml in diethyl ether. The balloon sections of the catheters are coated as described in the above examples; after removal from the coating solution, the balloons should be brought into a horizontal position and continuously be turned around their longitudinal axis as soon as possible.

## EXAMPLE 11

Epothilone B is dissolved in ethyl acetate at a concentration of 2 mg/ml; the solution is used to coat balloon catheters as described in the above examples.

## The invention claimed is:

1. A balloon catheter medical device that releases a drug by immediate release for the selective therapy of specific diseased tissue or an organ part to which said drug will bind, comprising such a drug which is lipophilic, water-insoluble and immediately releasable, adhered to a smooth surface of the balloon of said catheter that comes into contact with the diseased tissue or organ part, which adhered drug when pressed against said tissue or organ part at least for a short time, is immediately released into said tissue or organ part, wherein the concentration of said drug on said surface is up to 5 µg/mm<sup>2</sup>.

2. The device according to claim 1, wherein said balloon catheter comprises a stent.

3. The device according to claim 2, wherein a balloon with preformed longitudinal folds is coated with the drug, and the inclination of said folds to refold is not lost after inflation.

4. The device according to claim 2, wherein a balloon is coated with said drug and comprises smooth material to

US 8,257,305 B2

9

which said drug adheres sufficiently well to resist forces required for folding, essentially without damage.

5. The device according to claim 2, wherein only the area covered by folds is coated with the drug that was dried after application.

6. The device according to claim 1, wherein said balloon catheter does not comprise a stent.

7. The device according to claim 1, wherein the lipophilic drug is an inhibitor of cell proliferation or inflammatory processes, or an antioxidant.

8. The device according to claim 7, wherein the drug used is paclitaxel or other taxane, rapamycin, tacrolimus, a corticoid, a sex hormone, a statin, an epothilone, probucol, a prostacyclin, or an angiogenesis inducer.

9. The device according to claim 7, wherein the lipophilic drug is present as a dry solid or oil on the surface of the device.

10. The device according to claim 9, wherein the dosage form of the drug includes amorphous structures with particle sizes ranging from <0.1 micron to 5 microns that dissolve quickly due to their large surface area and despite the water-insolubility of the drug.

11. The device according to claim 1, wherein the lipophilic drug is embedded in a readily water-soluble matrix substance to achieve good adhesion to the surface of the device and improve absorption by the tissue.

12. The device according to claim 11, wherein said matrix substance is a low-molecular weight hydrophilic substance with a molecular weight <5000 D.

13. A medical device of claim 12 wherein said drug is paclitaxel and said device is an angioplasty balloon catheter having a smooth balloon surface.

14. The device according to claim 1, wherein the lipophilic drug is absorbed to particles of or applied to the surface of the device with, a low-molecular weight matrix.

15. The device according to claim 1, having a surface additionally coated with a substance that influences the gliding quality of the device or that prevents blood coagulation.

16. A medical device of claim 1 wherein said drug is paclitaxel and said device is an angioplasty balloon catheter having a smooth balloon surface.

17. A method for producing the device according to claim 1, comprising applying the lipophilic drug in a solution, suspension or emulsion medium using an immersion, spreading, or spraying process or an instrument which delivers a defined volume to the surface of the device to provide a coating and removing excess media and substances that adhere loosely to the surface.

18. The method according to claim 17, wherein the coating process is carried out repeatedly to achieve a reproducible increase of the drug content using the same or a different solution, suspension, or emulsion medium and/or excipient.

19. The method according to claim 18, wherein ethanol, isopropanol, ethyl acetate, diethyl ether, acetone, dimethyl sulfoxide, dimethyl formamide, glycerin, water or a mixture thereof is used as solution, suspension, or emulsion medium.

20. The method according to claim 17, wherein a balloon folded ready for use is used as the drug carrier coated prior to or after sterilization with or without a crimped-on stent.

21. The method according to claim 20, wherein the balloon is coated with the lipophilic drug in unfolded condition and then is folded with a lubricating tool optionally wetted with a biocompatible, gliding agent.

22. The method according to claim 17, wherein a stent is attached prior to or after coating of the balloon.

23. The method according to claim 17, wherein the completely coated device is sterilized using ethylene oxide.

10

24. A method of treating a vascular disease or circulation disturbance comprising administering a device of claim 1 to affected tissue.

25. A method of opening a passage in the body comprising administering a device of claim 1.

26. A balloon catheter having folds in its balloon, comprising a lipophilic, water-insoluble drug which binds to tissue, said drug being adhered to a smooth balloon surface in a fashion wherein it is immediately released upon coming into contact with said tissue, wherein the balloon area covered with folds is coated with said drug which has been dried after application, and wherein the concentration of said drug on said surface is up to 5  $\mu\text{g}/\text{mm}^2$ .

27. The balloon catheter according to claim 26, further comprising a stent, a needle or a guiding wire.

28. The balloon catheter according to claim 26, comprising in its finally folded state a balloon coated with a low-viscosity active agent solution of said drug, by immersing, spraying or applying via a volume measuring device.

29. The balloon catheter according to claim 26, wherein the lipophilic drug is an inhibitor of cell proliferation or an inflammatory process, or an antioxidant.

30. The balloon catheter according to claim 29, wherein the drug is paclitaxel or other taxane, rapamycin, tacrolimus, a corticoid, a sex hormone, a statin, an epothilone, probucol, a prostacyclin or an angiogenesis inducer.

31. The balloon catheter according to claim 29, wherein the lipophilic drug is present as a dry solid or oil on the surface of the balloon.

32. The balloon catheter according to claim 31, wherein the dosage form of the drug comprises amorphous structures with particle sizes ranging from <0.1 micron to 5 microns that dissolve fast due to their large surface area and despite the water-insolubility of the drug.

33. The balloon catheter according to claim 26, wherein said lipophilic drug is embedded in a readily water-soluble matrix substance to achieve good adhesion to the surface of the balloon and improved absorption by the tissue.

34. The balloon catheter according to claim 33, wherein said matrix substance is a low-molecular weight hydrophilic substance with a molecular weight <5000 D.

35. A balloon catheter of claim 34 wherein said drug is paclitaxel and said device is an angioplasty balloon catheter having a smooth balloon surface.

36. The balloon catheter according to claim 33, wherein said matrix substance is a contrast agent.

37. The balloon catheter according to claim 36, wherein said substance is an iodinated X-ray contrast agent.

38. The balloon catheter according to claim 37, wherein the drug is paclitaxel and the X-ray contrast agent is iopromide.

39. The balloon catheter according to claim 26, wherein said lipophilic drug is absorbed to a particle or applied to the surface of the device with a low-molecular weight matrix.

40. The balloon catheter according to claim 26, having a surface additionally coated with a substance that influences the glidability of the device or that prevents blood coagulation.

41. A balloon catheter of claim 26 wherein said drug is paclitaxel and said device is an angioplasty balloon catheter having a smooth balloon surface.

42. A method for producing the coated balloon catheter according to claim 26, comprising applying the lipophilic drug in a solution, suspension or emulsion medium using an immersion, spreading, or spraying process or a volume measuring device to the surface of a folded balloon, and removing excess media and substances that adhere loosely to the surface.

## US 8,257,305 B2

11

43. The method according to claim 42, wherein the coating process is carried out repeatedly to achieve a reproducible increase of the drug content using the same or a different solution, suspension, or emulsion medium and/or excipient.

44. The method according to claim 43, wherein ethanol, isopropanol, ethyl acetate, diethyl ether, acetone, dimethyl-sulfoxide, dimethylformamide, glycerol, water or a mixture thereof is used as solution, suspension, or emulsion medium.

45. The method according to claim 42, wherein a folded and substantially ready for use balloon is used as the drug carrier coated before or after sterilization with or without a crimped-on stent.

46. The method according to claim 42, wherein a stent is connected to the balloon catheter before or after coating.

47. The method according to claim 42, wherein the finally coated balloon catheter is sterilized using ethylene oxide.

48. A method for the treatment of a vascular disease or a dysfunction of circulation comprising administering a catheter of claim 26.

49. A method for opening a passage in the body comprising administering a catheter of claim 26.

50. A method for tumor treatment comprising administering a catheter of claim 26.

51. A balloon catheter medical device that releases a drug by immediate release for the selective therapy of specific diseased tissue or an organ part to which said drug will bind, comprising such a drug which is lipophilic, water-insoluble and immediately releasable, adhered to a surface of the balloon of said catheter that comes into contact with the diseased

12

tissue or organ part, which adhered drug when pressed against said tissue or organ part at least for a short time, is immediately released into said tissue or organ part, wherein the drug is adhered to said surface in a manner resulting in an amount of drug retained on said device of about 10% or less after a time period in which said balloon surface is in contact with said tissue of up to a few minutes, and wherein the concentration of said drug on said surface is up to  $5 \mu\text{g}/\text{mm}^2$ .

52. A balloon catheter of claim 51 wherein said drug is paclitaxel and said device is an angioplasty balloon catheter having a smooth balloon surface.

53. The device of claim 1 wherein the lipophilic drug is present as a dry solid on the surface of the device.

54. The device of claim 53 wherein the lipophilic drug is paclitaxel.

55. The device of claim 53 wherein the dried solid also comprises a contrast agent.

56. The device of claim 55 wherein the dried solid comprises paclitaxel and iopromide.

57. The catheter of claim 26 wherein the lipophilic drug is present as a dry solid on the surface of the device.

58. The catheter of claim 57 wherein the lipophilic drug is paclitaxel.

59. The catheter of claim 57 wherein the dried solid also comprises a contrast agent.

60. The catheter of claim 59 wherein the dried solid comprises paclitaxel and iopromide.

\* \* \* \* \*