



US008574312B2

(12) **United States Patent**
Moser et al.

(10) **Patent No.:** **US 8,574,312 B2**
(45) **Date of Patent:** **Nov. 5, 2013**

(54) **PROSTHETIC ANKLE JOINT MECHANISM**

(75) Inventors: **David Moser**, Hampshire (GB); **Fadi Abimosleh**, Springboro, OH (US); **Mir Saeed Zahedi**, London (GB); **Graham Harris**, Hampshire (GB); **Stephen Terry Lang**, Hampshire (GB); **Andrew Sykes**, Hampshire (GB)

2,699,554 A	1/1955	Comelli	
2,851,694 A *	9/1958	Capella Valenti	623/40
3,871,032 A	3/1975	Karas	
4,051,558 A	10/1977	Vallotton	
5,030,239 A	7/1991	Copes	
5,044,360 A	9/1991	Janke	

(Continued)

FOREIGN PATENT DOCUMENTS

(73) Assignee: **Blatchford Products Limited**, Hampshire (GB)

CN	101518473 A	9/2009
DE	2101303	6/1972

(Continued)

(*) Notice: Subject to any disclaimer, the term of this patent is extended or adjusted under 35 U.S.C. 154(b) by 195 days.

OTHER PUBLICATIONS

(21) Appl. No.: **11/956,391**

Anatomic and Biomechanical Characteristics of the Ankle Joint and Total Ankle Arthroplasty, Total Ankle Arthroplasty, Dec. 5, 2005, Springer Vienna, ISBN 978-3-211-21252 (print) 978-3-211-27254-1 (online), pp. 25-42.

(22) Filed: **Dec. 14, 2007**

(65) **Prior Publication Data**

US 2008/0262635 A1 Oct. 23, 2008

(Continued)

Related U.S. Application Data

(60) Provisional application No. 60/869,959, filed on Dec. 14, 2006.

Primary Examiner — David Isabella

Assistant Examiner — Jacqueline Woznicki

(74) Attorney, Agent, or Firm — Alston & Bird LLP

(51) **Int. Cl.**
A61F 2/64 (2006.01)

A61F 2/68 (2006.01)

(52) **U.S. Cl.**
USPC **623/47**; 623/49; 623/50

(58) **Field of Classification Search**
USPC 623/52, 47, 56
See application file for complete search history.

(56) **References Cited**


U.S. PATENT DOCUMENTS

37,637 A	2/1863	Parmelee	
2,657,393 A *	11/1953	Haller	623/26

(57) **ABSTRACT**

A self-aligning prosthetic foot and ankle assembly has an ankle unit pivotally mounting a foot component. The ankle unit contains a hydraulic piston and cylinder assembly having a piston which is linearly movable within a cylinder. The axis of the cylinder is coincident with a shin axis defined by a shin connection interface on the ankle unit. Bypass passages containing damping resistance control valves provide continuous hydraulic damping of dorsi and plantar ankle flexion, the unit being such that, over the major part of the range of damped movement, there is no resilient biasing in either the dorsi or the plantar direction. This confers a number of advantages, including stabilisation of standing, balance control, and improved stair-walking and ramp-walking.

22 Claims, 5 Drawing Sheets

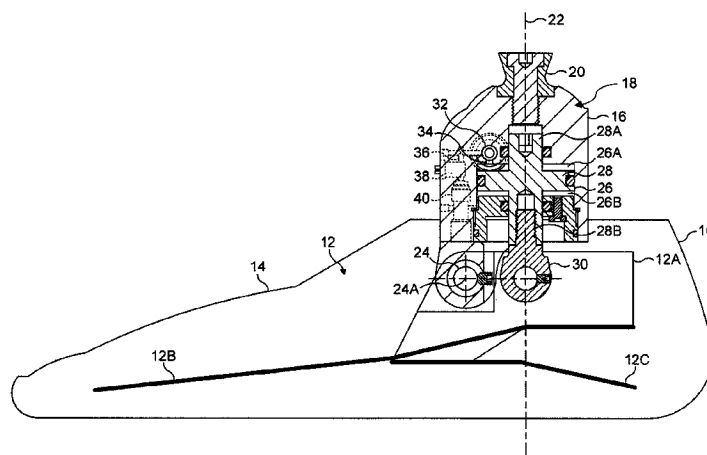

(56)

References Cited

U.S. PATENT DOCUMENTS

5,116,383	A	5/1992	Shorter et al.	
5,383,939	A *	1/1995	James	623/24
5,458,656	A *	10/1995	Phillips	623/27
5,957,981	A	9/1999	Gramnas	
6,033,440	A	3/2000	Schall et al.	
6,080,197	A	6/2000	Chen	
6,187,052	B1	2/2001	Molino et al.	
6,443,993	B1 *	9/2002	Koniuk	623/24
6,517,585	B1 *	2/2003	Zahedi et al.	623/24
6,863,695	B2	3/2005	Doddroe et al.	
7,985,265	B2	7/2011	Moser et al.	
2002/0052663	A1	5/2002	Herr et al.	
2002/0082712	A1 *	6/2002	Townsend et al.	623/52
2002/0120349	A1 *	8/2002	Phillips	623/35
2002/0138153	A1	9/2002	Koniuk	
2004/0044417	A1	3/2004	Gramnas	
2004/0054423	A1 *	3/2004	Martin	623/25
2004/0236435	A1	11/2004	Chen	
2005/0109563	A1	5/2005	Vitale et al.	
2005/0192677	A1	9/2005	Ragnarsdottir et al.	
2005/0267601	A1	12/2005	Chen	
2006/0069448	A1	3/2006	Yasui	
2006/0069449	A1 *	3/2006	Bisbee et al.	623/26
2006/0235544	A1 *	10/2006	Iversen et al.	623/26
2006/0249315	A1	11/2006	Herr et al.	
2007/0043449	A1 *	2/2007	Herr et al.	623/24
2008/0262635	A1	10/2008	Moser et al.	
2008/0281435	A1	11/2008	Abimosleh et al.	
2008/0300692	A1	12/2008	Moser	
2012/0130508	A1	5/2012	Harris	

FOREIGN PATENT DOCUMENTS

EP	0 549 855	B1	3/1996
EP	0 948 947		10/1999
EP	0 948 947	A2	10/1999
EP	1 068 844	A1	1/2001
GB	643734		9/1950
GB	2 328 160	A	2/1999
JP	59-189843	A	10/1984
JP	59183747		10/1984
JP	59189843		10/1984

JP	2001-514925	A	9/2001
JP	2004-506480	A	3/2004
JP	2008-536614	T	9/2008
JP	2009-515628	A	4/2009
WO	WO 93/06795	A1	4/1993
WO	WO 96/25898		8/1996
WO	WO 99/00075		1/1999
WO	WO 00/76429		12/2000
WO	WO 00/76429	A1	12/2000
WO	WO 02/15826	A1	2/2002
WO	WO 03/086245	A2	10/2003
WO	WO 2006/112774	A1	10/2006
WO	WO 2007/027808	A2	3/2007
WO	WO 2007/054736	A2	5/2007
WO	WO 2008/071975	A1	6/2008
WO	WO 2008/103917	A1	8/2008

OTHER PUBLICATIONS

Hydraulik Ankle Unit Manual; Mauch Laboratories, Inc.
 Search Report for Great Britain Application No. 1101893.4 dated May 11, 2011.
 Combined Search and Examination Report for Great Britain Application No. GB1201875.0 dated Apr. 12, 2012.
 International Search Report and Written Opinion for International Application No. PCT/US2008/054741, mailed Jul. 2, 2008.
 International Search Report and Written Opinion for International Application No. PCT/GB2012/000112, mailed May 5, 2012.
 Endolite Global—Echelon VT Foot—Prescription [online] retrieved May 7, 2012]. Retrieved from the Internet: <URL: http://www.endolite.co.uk/products/feet/echelon_vt/echelon_vt_foot.html> 1 page.
 United States Office Action for U.S. Appl. No. 13/364,786, dated May 22, 2013.
 Office Action for Japanese Application No. 2009-551033 dated Sep. 11, 2012.
 Morris, J.W., *Accelerometry—A Technique for the Measurement of Human Body Movements*, Journal of Biomechanics (1973) 726-736.
 Hayes, W. C. et al., *Leg Motion Analysis During Gait by Multiaxial Accelerometry: Theoretical Foundations and Preliminary Validations*, Journal of Biomechanical Engineering, vol. 105 (1983) 283-289.
 Office Action for U.S. Appl. No. 13/150,694; dated Dec. 14, 2012.

* cited by examiner

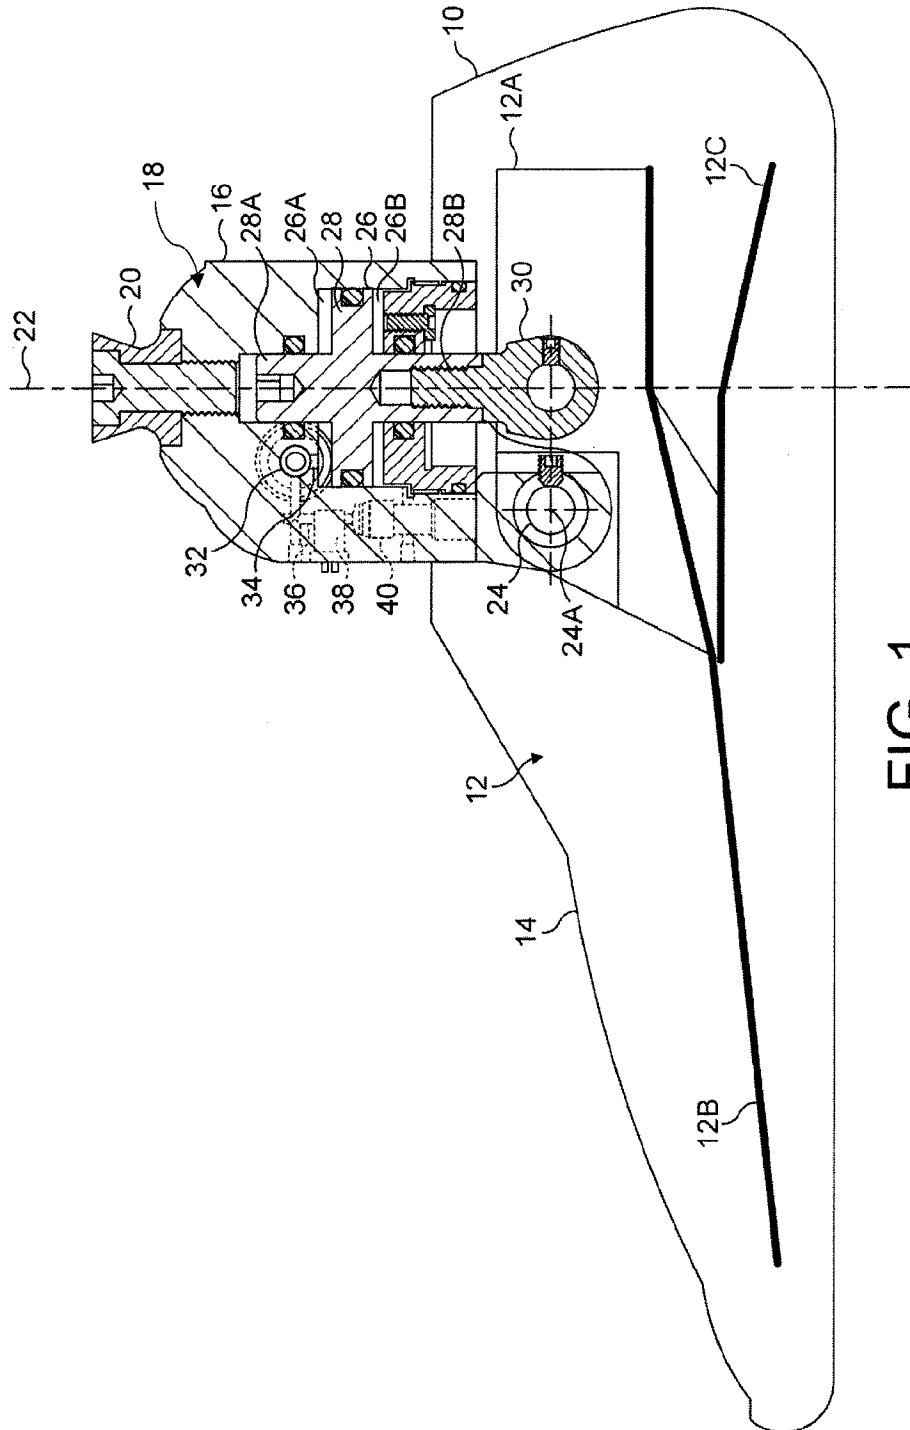


FIG. 1

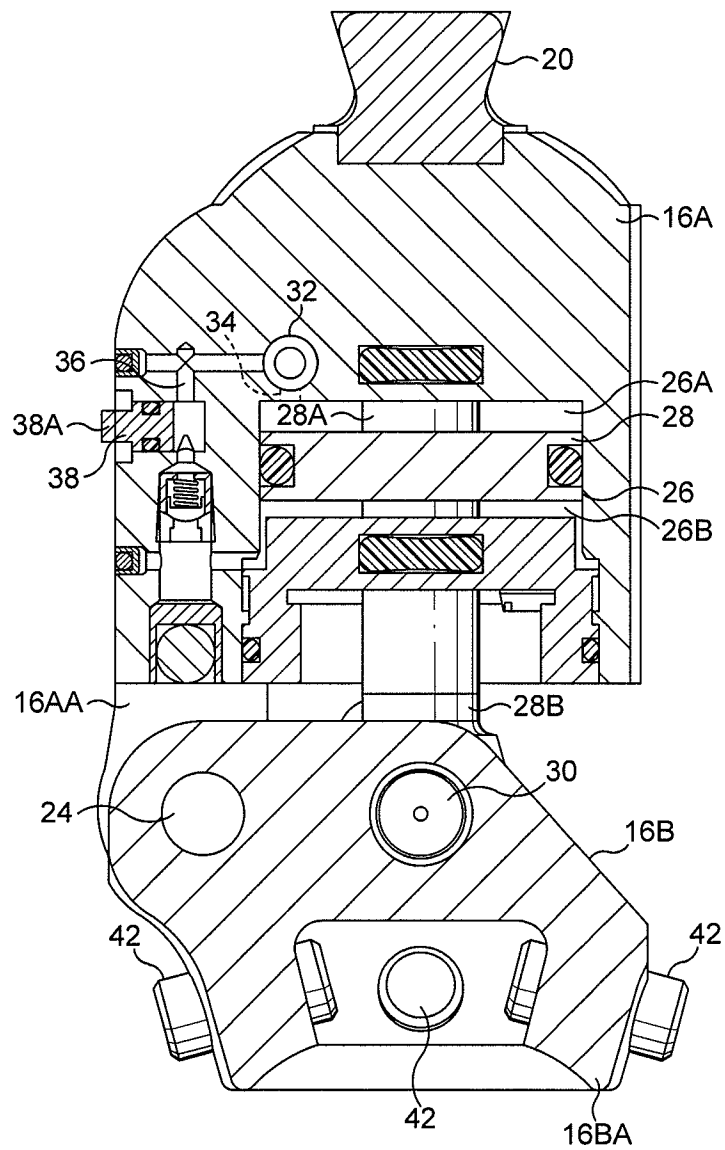


FIG. 2

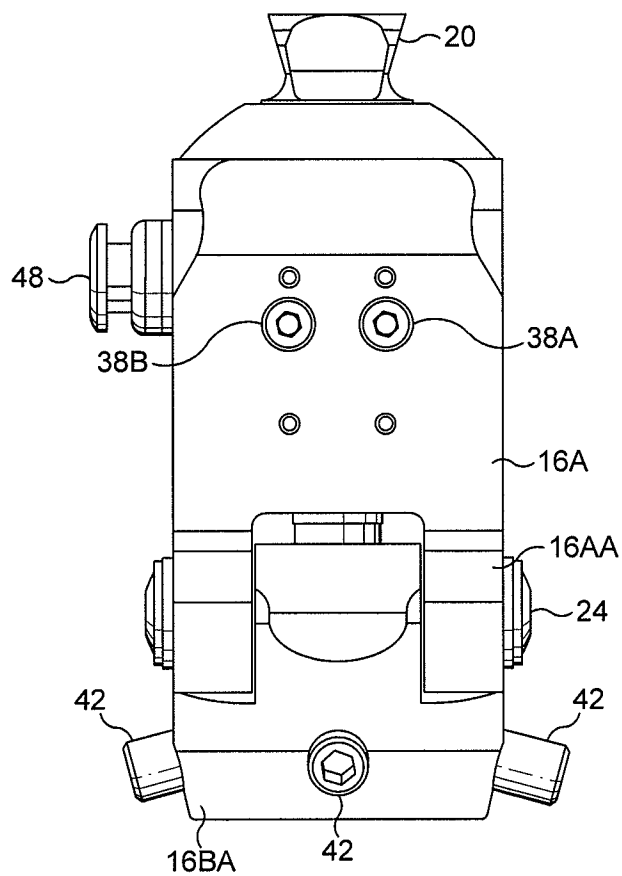


FIG. 3

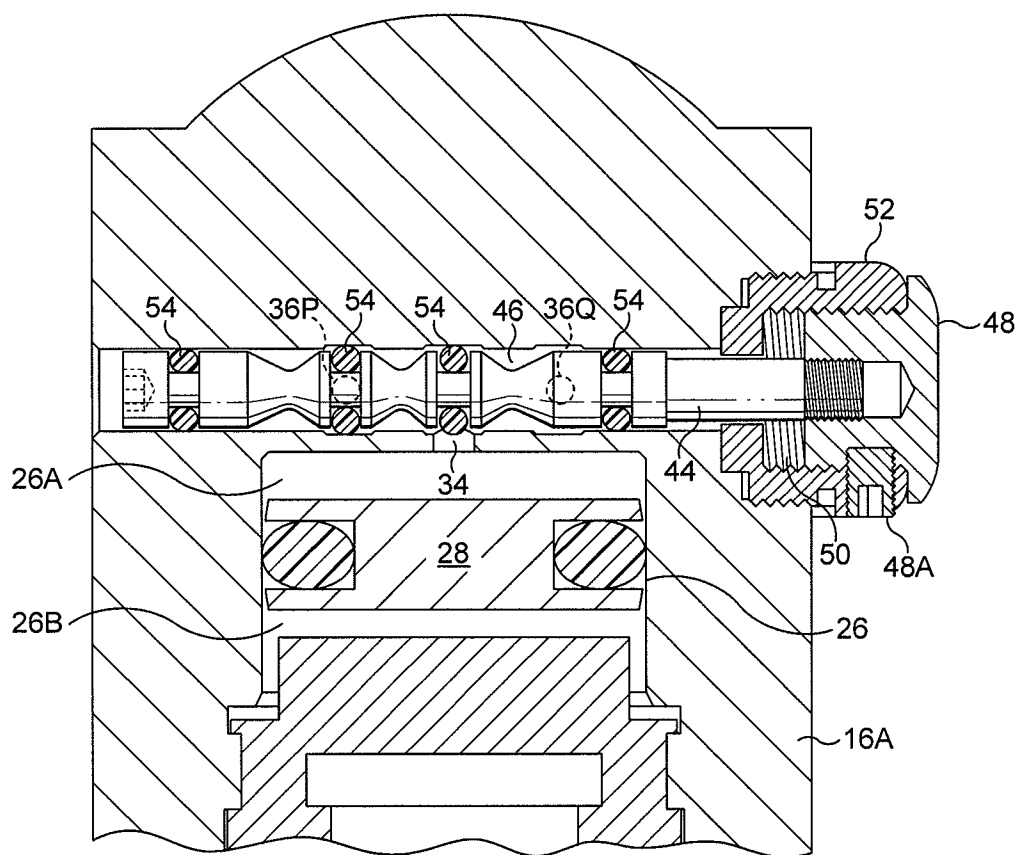


FIG. 4

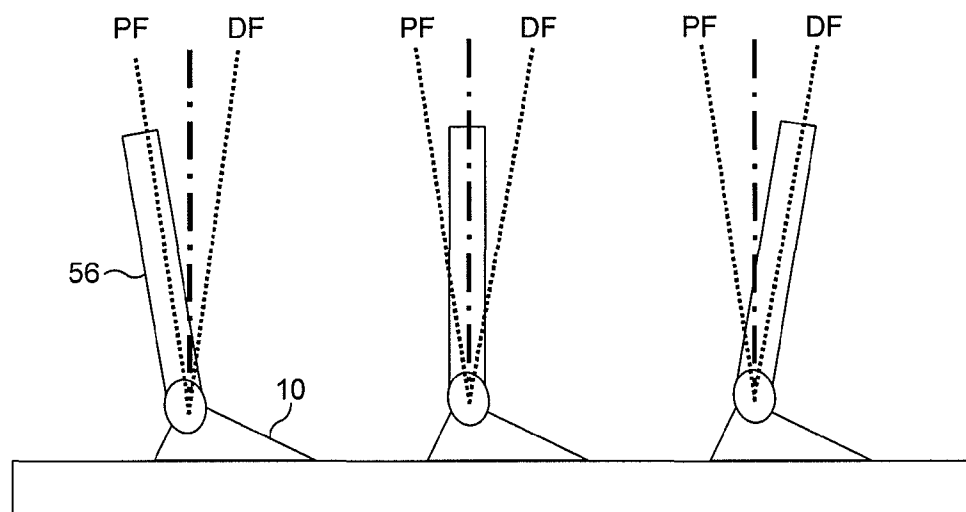


FIG. 5

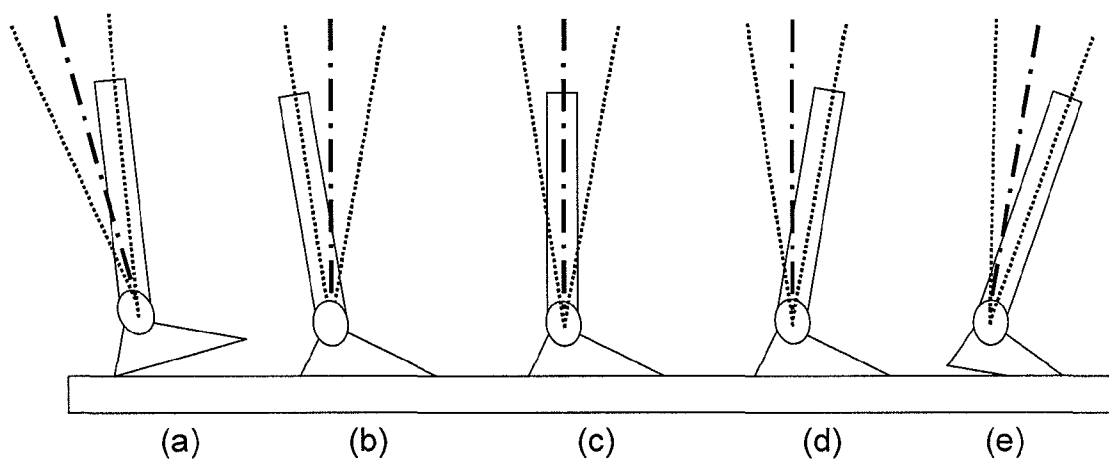


FIG. 6

1

PROSTHETIC ANKLE JOINT MECHANISM**CROSS-REFERENCE TO RELATED APPLICATION**

The present application claims the benefit of the filing date of U.S. Provisional Patent Application Ser. No. 60/869,959 filed Dec. 14, 2006, the entire disclosure of which is hereby incorporated herein by reference.

BACKGROUND OF THE INVENTION

This invention relates to a prosthetic ankle joint mechanism, to a lower limb prosthesis comprising a shin component, a foot component, and a joint mechanism interconnecting the shin and foot components, and to a prosthetic foot and ankle assembly. The joint mechanism is arranged to allow limited damped pivoting movement of the shin component relative to the foot component.

Current prosthetic foot and ankle systems are generally aligned for operation as fixed mechanical structures comprising elastic and deformable elements designed to provide stability during standing and walking and to return energy for propulsion into the swing phase of the walking cycle. However, such a device is often uncomfortable for the user whilst standing and whilst walking on ramps and stairs and walking at different speeds. Users have also experienced knee instability and difficulty in maintaining forward motion during roll-over of the foot while standing and walking on ramps and stairs, with consequent impairment of efficiency. These difficulties are particularly important for transfemoral amputees whose stance phase action is normally compromised by significantly reduced knee flexion and extension which would otherwise assist shock absorption and forwards propulsion during the stance phase.

An ankle joint mechanism allowing dynamic hydraulic control of the angular position of a prosthetic foot with respect to a shin component is disclosed in Mauch Laboratories, Inc., *Hydraulic Ankle Unit Manual*, March 1988. The shin component is attached to a vane piston housed in a fluid-filled chamber with a concave part-circular lower wall. A gravity-controlled ball rolls forwards and backwards on the wall according to the orientation of the foot to open or close a bypass passage in the piston. As a result, dorsi-flexion of the mechanism is prevented when the shin component is vertical, largely irrespective of whether the foot is horizontal or inclined downwardly or upwardly. Such a prosthesis also suffers partly from the disadvantages described above.

Amongst other known prosthetic ankle systems is that of U.S. Pat. No. 3,871,032 (Karas). This system contains a damping device having a dual piston and cylinder assembly with tappet return springs acting continuously to return the ankle to a neutral position. EP-A-0948947 (O'Byrne) discloses a prosthetic ankle having a ball-and-socket joint with a chamber filled with a silicone-based hydraulic substance, the joint having a visco-elastic response. In one embodiment, the chamber contains solid silicone rubber particles suspended in a silicone fluid matrix. US2004/0236435 (Chen) discloses a hydraulic ankle arrangement with adjustable hydraulic damping and resilient biasing members mounted anteriorly and posteriorly of an ankle joint rotation axis. In WO00/76429 (Gramtec), a leg prosthesis is described having an ankle joint allowing heel height adjustment by way of a hydraulic piston and linkage arrangement. Elastic components absorb shock

2

during walking. US2006/0235544 (Iversen et al) discloses a hydraulic ankle mechanism with a rotary vane.

BRIEF SUMMARY OF THE INVENTION

5

According to a first aspect of this invention, a prosthetic ankle joint mechanism provides a continuously hydraulically damped range of ankle flexion, the mechanism being constructed and arranged such that, over at least part of said range, the damping resistance is the predominant resistance to flexion. The mechanism preferably comprises a hydraulic linear piston and cylinder assembly. The piston may have distal connection means for pivotal connection to a foot component, the cylinder having proximal connection means for connection to a shin component. Typically, the piston and cylinder assembly has a central axis which is oriented such that when the mechanism is coupled to a prosthetic shin component, the central axis is substantially aligned with or parallel to a shin axis defined by the shin component.

To allow individual setting of dorsi and plantar-flexion damping resistances, the mechanism may have a valve arrangement controlling the flow of hydraulic fluid between chambers of the piston and cylinder on opposite sides of the piston, the valve arrangement preferably comprising first and second adjustable valves for dorsi-flexion and plantar flexion damping control respectively.

According to another aspect of the invention, a prosthetic ankle joint mechanism provides a continuously hydraulically damped range of ankle flexion, the mechanism being constructed and arranged such that, over at least part of the range, movement in the dorsi and plantar directions is substantially unbiased resiliently.

The invention also includes a prosthetic foot and ankle assembly comprising the combination of a foot component and, mounted to the foot component, an ankle joint mechanism having the features described above. It is preferred that the ankle joint mechanism includes flexion limiting means limiting dorsi flexion of the joint mechanism to a dorsi-flexion limit, the shin connection interface being arranged to allow connection of a shin component at different anterior-posterior tilt angles. These angles include angles resulting in the shin component having an anterior tilt of at least 3° with respect to the vertical when the joint mechanism is flexed to the dorsi-flexion limit. The dorsi-flexion limit advantageously corresponds to a predetermined orientation of the shin component interface relative to the foot component and may be defined by a mechanical end stop operative by the abutment of one part of the prosthetic foot and ankle assembly associated with the shin component interface against another part of the assembly associated with the foot component. Conveniently, the end stop is defined by the piston of the piston and cylinder assembly abutting an end wall of the cylinder.

In the preferred embodiment of the invention described hereinafter, the range of damped ankle flexion is fixed. Nevertheless, the above-mentioned dorsi-flexion limit may be adjustable over at least a range of anterior-posterior tilt angles from 3° to 6°. In another embodiment, the range of damped flexion may alter when the dorsi-flexion limit is adjusted, but once the adjustment has been made, the range of damped flexion is, likewise, fixed from step to step.

The assembly may be arranged such that the relative position of the foot component and the shin connection interface at the dorsi-flexion limit is defined independently of the orientation of the assembly in space.

Adjustment of the shin axis orientation in the anterior-posterior direction with respect to the foot component may be

3

performed using at least one conventional pyramid alignment interface, preferably the shin component interface.

The above-described prosthesis, in which the ankle allows dorsi-plantar flexion over a limited range of movement with largely damped, as opposed to resilient, resistance to motion results in an ankle which is able easily to flex under load according to changing activity requirements without generation of high reaction moments which would otherwise cause discomfort and compromise the function of the prosthesis. Providing damped and substantially unbiased movement means that the ankle thereby functions in a way such that it remains in its last loaded orientation, having no re-alignment capability once the foot is unloaded. This feature is advantageous to assist foot clearance during the swing phase.

By arranging for the position of the foot component or the foot component interface relative to the shin connection interface at the dorsi-flexion limit to be defined independently of the orientation of the assembly in space, and by using gravity-independent determination of the dorsi-flexion limit, the need for a gravity-dependent valve system with an end-stop corresponding to vertical orientation of the shin axis is avoided. The prosthesis described above allows set-up flexibility to alter the dynamics of roll-over through selection of different toe spring stiffnesses. The range of yielding motion can be altered by altering the relative alignment of the foot and shin components. Allowing the shin axis to move to the anterior of the vertical position is particularly advantageous during stair and ramp walking activities.

The conventional approach of maximising energy storage and return has produced designs in which the ankle has a high elastic stiffness at all times. Reducing stiffness in the manner proposed in accordance with the present invention greatly improves comfort for the user as well as helping to preserve forwards momentum of the upper body and thus locomotion efficiency. Reaction moments about the ankle are largely dissipated with the result that voluntary control and proprioception of the knee and hip in BK (below-knee) amputees, in particular, is improved.

According to a further aspect of the invention, there is provided a prosthetic foot and ankle assembly comprising the combination of an ankle joint mechanism as described above, together with a prosthetic energy-storing foot which is resiliently deformable to allow dorsi-flexion of at least an anterior portion of the foot relative to an ankle-mounting portion of the foot.

The invention also includes a lower limb prosthesis comprising a shin component defining a shin axis, a foot component, and an ankle joint mechanism as described above, the ankle joint mechanism coupling the shin component to the foot component, wherein at least one of the foot component and the shin component includes a resilient section allowing resilient dorsi-flexion of at least an anterior portion of the foot component relative to the shin axis. The foot component may comprise an energy-storing spring arranged to be deflected when a dorsi-flexion load is applied to the foot anterior portion. Alternatively, the prosthesis may include a resilient section associated with the coupling of the foot component and the ankle joint mechanism, allowing a degree of resilient dorsi-flexion. As another alternative, there may be a resilient section associated with the coupling of the shin component to the ankle joint mechanism.

Another aspect of the invention resides in a prosthetic foot and ankle assembly comprising the combination of an ankle joint mechanism and a prosthetic foot having an anterior portion, a posterior portion and an ankle-mounting portion, wherein the assembly constitutes a Maxwell-model damper/spring combination of which the damper element is said ankle

4

joint mechanism and the spring element is a spring component arranged in series with the ankle joint.

Described below is a lower limb prosthesis comprising a shin component defining a shin axis, a foot component, and a joint mechanism interconnecting the shin and foot components and arranged to allow limited damped pivoting of the shin component relative to the foot component about a medial-lateral joint flexion axis during use, wherein the mechanism comprises: a piston and cylinder assembly the piston of which is movable so as to define a variable-volume fluid-filled chamber of the assembly, fluid being admitted to or expelled from the chamber through at least one damping orifice as the relative orientation of the shin and foot components varies with flexion of the joint mechanism; and flexion limiting means limiting dorsi-flexion of the joint mechanism to a dorsi-flexion limit corresponding to orientation of the shin component with the shin axis tilted anteriorly with respect to the vertical by at least 3 degrees. The joint mechanism is preferably arranged such that damped relative pivoting of the shin component and the foot component is allowed over an angular range between dorsi- and plantar-flexion limits, the dorsi-flexion limit being adjustable to different anterior tilt settings of the shin axis with respect to the foot component. In particular, the angular range encompasses a foot-flat, shin-axis-vertical state with the permitted degree of shin axis tilt being adjustable to different values to the anterior of the vertical.

In the preferred embodiment of the invention, the joint mechanism has a first part associated with the shin component and a second part associated with the foot component, these two parts being pivotally interconnected with the connection defining a joint flexion axis. One of the two parts includes the chamber of the piston and cylinder assembly and the other is pivotally connected to the piston, the mechanism being arranged such that the dorsi-flexion limit is defined by a mechanical stop limiting relative rotation of the first and second parts. This mechanical stop may be the abutment of the piston with an end surface of the chamber. A cushioning spring or pad may be applied to the top surface of the piston or to the opposing chamber surface in order to increase the resistance to dorsi-flexion as the dorsi-flexion limit is approached.

As for the ability to preset the dorsi-flexion limit, this may be facilitated in a number of ways. For instance, the limit may be set by an adjustable anterior-posterior tilt alignment interface, typically between the joint mechanism and a shin component such as a shin tube. The interface may be of the well-known inverted pyramid construction as described above. Alternatively, the interface may be provided between the joint mechanism and a foot component. Again this may be of inverted-pyramid construction. Another possibility is a lockable pivot joint for connecting the foot component to the joint mechanism, having an adjustment axis running in the medial-lateral direction. As a further alternative, an adjustable end stop may be provided in the piston and cylinder assembly, or the connection between the piston and one of the components of the mechanism mounting the foot component or the shin component may be adjustable to alter the range of displacement of the piston in the chamber of the assembly with respect to the angular range of movement of the foot component relative to the shin component.

The preferred joint mechanism includes two passages in communication with the above-mentioned chamber of the piston and cylinder assembly, each containing a respective non-return valve, one oriented to prevent the flow of fluid from the chamber through its respective passage and the other oriented to prevent the admission of fluid to the chamber

5

through the other passage, so that one permits fluid flow when the joint mechanism is flexing in the direction of dorsi-flexion while the other passage permits the flow of fluid when the joint is flexing in the direction of plantar-flexion. Preferably, both passages have respective adjustable-area damping orifices to allow the degree of damping to be tuned to the user's requirements.

It is preferred that the piston and cylinder assembly is a hydraulic piston and cylinder assembly, although it is possible to use a pneumatic assembly.

A locking device may also be provided for locking the joint mechanism against pivoting at any of a number of positions of the foot component relative to the shin component. Typically this is performed using a manually or electromechanically operated valve which interrupts the flow of fluid to or from the above-mentioned chamber of the piston and cylinder assembly through the bypass passages. The locking device comprises a control member having two positions, one in which the joint mechanism operates in a yielding mode and one in which it operates in a locked mode. Retaining means are provided for retaining the control member in either of the two positions, e.g. a spring biasing the control member into one position and a detent, latch or lock for keeping the control member in the other position.

The invention also includes a prosthetic ankle unit comprising a foot connection interface, a shin connection interface pivotally connected to the foot connection interface to allow flexion of the unit, a piston and cylinder assembly having a piston that is movable in a fluid-filled chamber of the assembly, the piston being associated with one of the interfaces and the chamber with the other so that when the shin connection interface pivots relative to the foot connection interface, the piston moves in the chamber, fluid being admitted to or expelled from the chamber through at least one damping orifice according to the direction of flexion of the unit, wherein the unit further comprises flexion limiting means limiting dorsi-flexion of the unit to a dorsi-flexion limit corresponding to a selected angular position of the interfaces relative to each other, and wherein at least one of the connection interfaces is configured to allow anterior-posterior tilt adjustment.

The invention will be described below by way of example with reference to the drawings.

BRIEF DESCRIPTION OF THE DRAWINGS

In the drawings:

FIG. 1 is a cross-section of a foot-ankle prosthesis in accordance with the invention, including a first ankle unit, sectioned on a central anterior-posterior (AP) plane;

FIG. 2 is a cross-section of an alternative ankle unit for use in a prosthesis in accordance with the invention, sectioned on an AP in front of the central AP plane;

FIG. 3 is an anterior elevation of the ankle unit of FIG. 2;

FIG. 4 is a detailed cross-section, taken on a medial-lateral plane, of the ankle unit of FIG. 2, showing a locking valve;

FIG. 5 is a diagram illustrating the ankle yielding range afforded by a prosthesis in accordance with the invention; and

FIG. 6 is a diagram illustrating operation of a prosthesis in accordance with the invention during walking.

DETAILED DESCRIPTION OF THE DRAWINGS

Referring to FIG. 1, an foot-ankle prosthesis in accordance with the invention has a foot component 10 with a foot keel 12 comprising a rigid carrier 12A, and a toe spring 12B and a heel spring 12C which are independently coupled to the car-

6

rier 12A. The keel 12 is a one-piece component made from a carbon fibre composite material and is surrounded by a foam cosmetic covering 14.

Mounted to the foot keel 12 is an ankle unit 16 comprising a joint mechanism 18 and a shin connection interface 20. The shin connection interface 20 defines a shin connection axis 22. The mounting of the ankle unit 16 to the foot keel 12 is by way of an ankle flexion pivot 24 defining a flexion axis 24A running in a medial-lateral direction to the anterior of the shin connection axis 22.

The body of the ankle unit 16 forms the cylinder of a piston and cylinder assembly having a piston 28 with upper and lower piston rods 28A, 28B, the lower piston rod being pivotally connected to the foot keel 12 at a second pivotal connection 30, this second pivotal connection defining a second medial-lateral axis which is spaced, in this case posteriorly, from the flexion axis 24A. It will be seen that as the body 16 of the ankle unit pivots about the flexion axis 24A, the piston 28 moves substantially linearly in the cylinder 26.

The cylinder 26 of the piston and cylinder assembly is divided into upper and lower chambers 26A, 26B. These chambers are linked by two bypass passages in the ankle unit body 16, one of which is visible in FIG. 1 where it is shown by dotted lines since it is behind the sectioning plane of the drawing. The other passage does not appear in FIG. 1 since it is located in front of the sectioning plane. However, its configuration is almost identical, as will be described below. These two bypass passages communicate with the upper chamber 26A of the cylinder via a locking valve 32, described in more detail below, and a common linking passage 34 which opens into the upper chamber 26A.

The two bypass passages, one of which, 36, is shown in FIG. 1, each contain a damping resistance control valve constituting a manually adjustable area orifice 38 and a non-return valve 40. This adjustable-area orifice and the non-return valve 40 are arranged in series in the bypass passage 36 between the locking valve 32 and the lower chamber 26B.

The bypass passage 36 appearing in FIG. 1 has its non-return valve 40 oriented to allow the flow of hydraulic fluid from the lower chamber 26B to the upper chamber 26A. The other bypass passage (not shown) has its non-return valve oriented in the opposite direction. Accordingly, one of the passages 36 is operative during dorsi-flexion and the other during plantar-flexion. When the locking valve 32 is open, continuous yielding movement of the foot component 10 relative to the ankle unit 16 about the flexion axis 24A is possible between dorsi-flexion and plantar-flexion limits defined by the abutment of the piston with, respectively, the lower wall and the upper wall of the cylinder 26. The level of damping for dorsi-flexion and plantar-flexion is independently and manually presettable by the respective adjustable-area orifices.

The shin connection interface 20 is conventional, being of pyramid construction. Typically, a tubular shin component is mounted to the shin connection interface 20, the shin component having, at its distal end, an annular female pyramid receptacle having alignment screws, as well known to those skilled in the art, for adjusting the orientation of the shin component relative to the ankle unit 16. At a neutral alignment position, the axis of the shin component (the shin axis) is coincident with the shin connection axis 22 (shown in FIG. 1). When the shin component is affixed to the ankle unit 16 in this neutral position, the limit of dorsi-flexion of the ankle-foot prosthesis, defined by the abutment of the piston 28 with the lower wall of the cylinder 26 corresponds to an anterior tilt of the shin axis relative to the vertical when the user stands on a horizontal surface. The plantar flexion limit, defined by

7

abutment of the piston **28** with the upper wall of the cylinder **26** corresponds to a posterior tilt of the shin axis.

In this embodiment, the anterior and posterior tilt angles of the shin connection axis **22** at the dorsi-flexion and plantar-flexion limits are 4 degrees (anterior) and 8 degrees (posterior) respectively with respect to the vertical.

In this embodiment, the mechanical end-stops represented by the abutment of the piston **28** with the lower and upper cylinder walls define a yield range over which the ankle-foot prosthesis is free to flex during locomotion and during standing, providing the locking valve **32** is open. Alteration of the shin component alignment at the shin connection interface **20** does not alter the angular magnitude of the yielding range because it is governed by the piston stroke, but it does alter the position of the limits with respect to the vertical.

It will be understood, therefore, that the angular range magnitude is fixed by the construction and geometry of the ankle-foot prosthesis and its hydraulic joint mechanism. The degrees of dorsi-flexion and plantar-flexion respectively are altered by the alignment of the shin component connection, as described above. It will be understood that alternative alignment interfaces can be used to adjust the positions of the dorsi-flexion and plantar-flexion limits. For instance, an anterior-posterior tilt alignment interface may be provided between the ankle unit **16** and the foot keel **12**. Such an interface is provided by a second embodiment of the invention, as will now be described with reference to FIGS. **2** and **3**.

Referring to FIG. **2**, this second embodiment of the invention takes the form of a two-part ankle unit having an ankle unit body **16A** which, as before, mounts a shin connection interface **20** for adjustable connection to a shin component (not shown), and a foot mounting component **16B** which incorporates a foot connection interface for receiving a pyramid connector of the known kind on a foot keel (not shown). The joint mechanism is identical to that described above with reference to FIG. **1** with the exception that the flexion and piston rod connection pivots **24**, **30** are housed in the foot mounting component **16B** rather than directly in the keel of a prosthetic foot. In the case of FIG. **2**, the drawing is a cross-section on a vertical anterior-posterior plane parallel to but spaced from the axis of the shin connection interface **20** and the cylinder **26**. Consequently, the bypass passage permitting hydraulic fluid flow from the lower chamber **26B** to the upper chamber **26A** of the cylinder **26** (corresponding to dorsi-flexion, i.e. clockwise rotation of the foot mounting component **16B** relative to the ankle unit body **16A** about the pivot **24**) appears in full lines, whereas the common linking passage **34** between the control valve **32** and the upper chamber **26A** is shown with dotted lines.

It will be understood that the non-return valve **40** has a counterpart non-return valve in the bypass passage (not shown) allowing for plantar flexion, but that the orientation of that counterpart valve is reversed from that shown in FIG. **2**, as described above with reference to FIG. **1**.

For the avoidance of doubt, it should be pointed out that the bores in the ankle unit body **16A** which house the upper and lower piston rods **28A**, **28B** provide sufficient clearance around the piston rods to allow a limited degree of rocking of the piston **28** and piston rods **28A**, **28B** relative to the cylinder as the foot mounting component **16B** rotates with respect to the ankle unit body **16A**. The periphery of the piston **28** is shaped so as to have an arcuate cross-section, also for this reason. The same features are present in the ankle unit of FIG. **1**.

The distal part of the ankle unit body **16A** is in the form of a trunnion **16AA** housing pivot axles of the flexion pivot **24**

8

and the piston rod connection pivot **30**. The foot mounting component **16B** has an integral annular female pyramid alignment coupling **16BA**. This annular pyramid connector includes four screws **42**, three of which are shown in FIG. **2**.

The ankle unit trunnion **16AA** is shown more clearly in FIG. **3**. Also visible in FIG. **3** are two adjustment screws **38A**, **38B** which are accessible on the anterior face of the ankle unit body **16A**. These form part of the adjustable-area orifices or flow resistance adjusters, one of which appears as valve **38** in FIG. **2**, and permit manual adjustment of damping resistance in the dorsi- and plantar-flexion directions respectively.

Referring now to FIG. **4**, which is a partial cross-section of the ankle unit on a medial-lateral plane containing the axis of the locking valve **32**, this locking valve is a spool valve having a spool member **44** which is slidable in a spool valve bore **46**. The bore has three ports. A first port is that of the common linking passage **34** communicating with the upper chamber **26A** of the cylinder **26**. Second and third ports **36P**, **36Q**, offset medially and laterally with respect to the common passage **34**, provide for communication with the bypass passages **36** (see FIG. **2**).

At one end of the spool member **44**, there is a manually operable pushbutton **48**, which, when pushed against the outward biasing force of a stack **50** of spring washers encircling the spool member within a pushbutton housing **52**, moves the spool member **44** to its open position, as shown in FIG. **4**.

The spool valve bore **46** has three enlarged sections of increased diameter in registry, respectively, with the three ports described above. The spool member **44** has four full-diameter sections, with sealing rings **54**, which are a sliding fit within the bore **46**. When the spool member **44** is in its open position, as shown in FIG. **4**, two of these full-diameter sections and their corresponding sealing rings **54** are in registry with the enlarged sections of the spool valve bore **46**, thereby allowing fluid flow between the bypass passage ports **36P**, **36Q** and the common passage **34** communicating with the upper chamber **26A** of the cylinder **26**. Conversely, when the push button **48** is released, the spool member **44** moves to bring the above-mentioned full-diameter portions and their respective sealing rings **54** into registry with the non-enlarged sections of the spool valve bore **46** on each side of the port to the common passage **34**, thereby preventing fluid flow between the upper cylinder chamber **26A** and the bypass passage ports **36B**, **36Q**. It follows that when the pushbutton **48** is released, the ankle unit is hydraulically locked at whichever flexion angle existed at the moment of release. The pushbutton **48** has a projecting stud **48A** which engages a detent recess in the push button housing **52** when the pushbutton is rotated, allowing the pushbutton to be maintained in its depressed position. This is the normal position of the spool valve, in which flow of hydraulic fluid through the bypass passages is **36** (FIG. **2**) is allowed, with the result that the ankle unit allows yielding dorsi- and plantar-flexion.

The same locking valve arrangement is present in the ankle unit of the foot-ankle prosthesis described above with reference to FIG. **1**.

Whether the ankle unit is in the form of a two-part assembly for detachable mounting to a foot component, as described above with reference to FIGS. **2**, **3** and **4**, or in the form of an ankle unit directly pivotally mounted to a prosthetic foot, as described above with reference to FIG. **1**, the joint mechanism allows yielding ankle flexion as shown diagrammatically in FIG. **5**. The dotted lines denote plantar-flexion (PF) and dorsi-flexion (DF) limits of a mechanical hydraulic yielding range of flexion of a shin component **56** with respect to a foot component **10**. The magnitude of the

angular range is fixed by the geometry of the joint mechanism and its damping piston and cylinder assembly. Although in these preferred embodiments, the range magnitude is fixed, the position of the limits with respect to a neutral position indicated by the chain lines in FIG. 5 can be altered by adjusting the alignment of the shin component relative to the foot component using one of the alignable connection interfaces described above. In this way, the flexion range may be biased anteriorly or posteriorly from the position shown in FIG. 5 to create a larger range of motion in either the PF or DF direction. Typical alignment settings result in a dorsi-flexion limit at 2 degrees to 6 degrees tilt anteriorly with respect to the neutral axis, dependent on the foot toe spring stiffness in particular, and the plantar flexion limit at 4 degrees to 10 degrees tilt posteriorly with respect to the neutral axis (shown by the chain lines in FIG. 5).

Providing the manual hydraulic lock is not activated, the unit continuously allows yield in the dorsi direction (and plantar direction) up to the preset dorsi-flexion limit during walking and standing.

The applicants have found that providing a yielding ankle with minimal, preferably zero elastic biasing in the dorsi- or plantar directions, and with flexion limits set within the above ranges, provides advantages during stair walking and ramp walking activities, and during standing. In the normal body, the biomechanics of standing balance control are characterised by the natural balancing of external moments between joint centres of rotation. The geometrical position of the joint centres of rotations and the relative position of the body centre of gravity and the reaction vector are important for stabilising action. Limb stability with a prosthetic limb is primarily dependent on geometry, not muscle-induced internal moments. Consequently, standing can be achieved for long periods with minimal muscular effort. A small amount of cyclical postural sway of the upper body also helps to create stability. It follows that natural standing posture and balance control can be achieved with joints exhibiting low levels of internal resistive torque, the position of the ground reaction vector relative to the hip, knee and ankle joints being the main source of limb stability. Allowing yield in a prosthetic ankle in the manner provided by the ankle-foot prosthesis described above aids this function for a lower limb amputee.

The dynamic action of a lower limb prosthesis having the features described above during the stance phase of walking is now described with reference to FIG. 6. At heel strike (a), the ankle is in a dorsi-flexed state from the roll-over actions of the previous step. As the foot moves towards the flat-foot state (b), the ankle plantar-flexes under the action of the foot heel spring and hydraulic yield at the ankle. In general, plantar-flexion at the ankle does not reach the plantar-flexion limit imposed by the joint mechanism of the prosthesis at this stage. During roll-over (c), the ankle begins to dorsi-flex by way of the hydraulic yield afforded by the prosthesis, providing a smooth roll-over action, preserving body momentum, and improving knee function. Towards the end of the roll-over phase (d), the dorsi-flexion limit imposed by the joint mechanism is reached. Once this happens, mechanical energy is directed into the keel of the foot (e) to provide energy return for push-off. The swing phase is initiated with the foot oriented at the dorsi-flexion end-stop to provide toe clearance during the swing phase.

In summary, the prosthesis described above is an foot-ankle system that is continuously allowed to yield over a limited range in plantar- and dorsi-flexion. The yielding action is provided by a hydraulic damper coupled to conventional foot elements (i.e. keel, carrier and independent carbon fibre composite heel-toe springs). The ankle is, therefore, free

to flex continuously over a limited plantar- and dorsi-flexion range via the hydraulic damper with minimal interference from elastic elements during walking and standing. During standing, the relative positions of the hip, knee and ankle joint centres are such that substantially normal standing postures can be maintained, the moments about each joint being automatically balanced thereby creating limb stability. Moreover, the self-aligning action of the foot-ankle system facilitates improved control of energy transfer between limb segments during locomotion, the user's hip joint being the main driver and the knee joint being the main facilitator of mechanical energy transfer. This biomimetic method of stabilisation of standing stability and balance control has a further advantage in that, while standing on ramps, owing to the yielding action of the hydraulic components, there are no significant reaction moments generated around the ankle which may cause imbalance between joints and discomfort. Since, owing to the limited range of hydraulic yielding, the ankle is free to move, adaptation for walking and standing on inclined surfaces and changes to footwear with various heel heights is achieved automatically. A further advantage of the system is a smoother more progressive transition during roll-over over a variety of terrains.

Although a pneumatic piston and cylinder assembly can be used in place of a hydraulic one, the hydraulic variant is preferred.

The preferred construction includes an alignment adaptor to allow setting and adjustment of the plantar-flexion and dorsi-flexion hydraulic yield limits. Such adjustment allows the prosthetist to provide for balancing of limb moments during standing.

The degree of resistance to flexion in the dorsi-direction or plantar-direction is manually adjustable (e.g. by rotation of flow control valve elements using a screwdriver). The control valves for controlling hydraulic resistance may, in an alternative embodiment, be replaced by a single adjustable control valve in a common bypass passage, supplemented, if necessary, by a second control valve in a branch passage.

In addition, the joint provided by the ankle-foot system may be hydraulically locked, preferably manually, but also, for instance, remotely in real time using an electrically controlled valve, preferably operated wirelessly via a key fob.

The dorsi-flexion end-stop may be cushioned, e.g. by inserting a compression spring on the upper cylinder wall or on the upper face of the piston. Alternatively, a resilient elastomeric or felt pad may be provided on one of these surfaces.

A further variation is the substitution of a hydraulic dorsi-flexion end stop in place of an end-stop determined by abutment of components of the joint mechanism. In this case the port via which the relevant bypass passage communicates with the chamber 26B (FIG. 2) of the piston and cylinder assembly may be located in the cylinder side wall of the cylinder above the lower wall of the lower chamber 26B so that as a piston 28 moves with dorsi-flexion of the mechanism, it covers the port thereby preventing further movement. The port may be shaped or divided into two or more openings into the chamber so that the resistance to dorsi-flexion increases as the dorsi-flexion limit is approached, providing a hydraulic cushion. A similar hydraulic stop may be provided by means of a port in the upper chamber 26A.

In summary, the preferred foot and ankle system as described has a linear piston arrangement for the simple control of a hydraulic damping range. There is no need for a pendulum as in some prior art arrangements, nor for electronic control at every step. The damping range is set mechanically, the linear piston arrangement being preferred for simplicity and reliability. Independent dorsi-flexion and

11

plantar-flexion valve adjustment is provided, allowing improved setup and customisation of foot performance to suit the requirements of individual amputees. The preferred foot and ankle combination represents a visco-elastic structure according to the Maxwell model, i.e. the damper of the ankle joint mechanism acts in series with the resilient part of the foot. The hydraulic damping is active on a step-by-step basis, as opposed to being substantially locked on some steps.

What is claimed is:

1. A prosthetic foot and ankle assembly comprising the combination of:

a foot component, and

an ankle joint mounted to the foot component, the ankle joint comprising:

a joint mechanism providing resistance to ankle flexion, wherein the joint mechanism is constructed and arranged such that during walking said resistance is predominantly provided by hydraulic damping whenever the ankle joint is flexed in both dorsi- and plantar-flexion directions.

2. A prosthetic foot and ankle assembly according to claim 1, further comprising a shin connection interface, wherein said joint mechanism includes a flexion limiter limiting dorsi-flexion of the joint mechanism to a dorsi-flexion limit, and wherein the shin connection interface is arranged to allow connection of a shin component at different anterior-posterior tilt angles, including angles resulting in the shin component having an anterior tilt of at least 3 degrees with respect to the vertical when the joint mechanism is flexed to the dorsi-flexion limit.

3. A prosthetic foot and ankle assembly according to claim 1, further comprising a shin connection interface, wherein the joint mechanism includes a flexion limiter limiting dorsi-flexion of the joint mechanism to a dorsi-flexion limit, and wherein the assembly is arranged such that the dorsi-flexion limit corresponds to a predetermined relative orientation of the shin component interface relative to the foot component.

4. A prosthetic foot and ankle assembly according to claim 3, wherein the dorsi-flexion limit is defined by a mechanical end-stop operative by the abutment of one part of the assembly associated with the shin component interface against another part of the assembly associated with the foot component.

5. A prosthetic foot and ankle assembly according to claim 4, wherein the joint mechanism comprises a hydraulic linear piston and cylinder assembly, wherein the piston has a distal connection and the cylinder has a proximal connection, and wherein the end stop is defined by the piston and an end wall of the cylinder.

6. A prosthetic foot and ankle assembly according to claim 1, further comprising a shin connection interface, wherein said joint mechanism includes a flexion limiter limiting dorsi-flexion of the joint mechanism to a dorsi-flexion limit, and wherein the assembly is arranged such that the relative position of the foot component and the shin connection interface at the dorsi-flexion limit is defined independently of the orientation of the assembly in space.

7. A prosthetic foot and ankle assembly according to claim 1, arranged such that the resistance to flexion of said joint mechanism in a direction of dorsi-flexion is adjustable.

8. A prosthetic foot and ankle assembly according to claim 1, having at least one pyramid alignment interface allowing adjustment of shin axis orientation in an anterior-posterior direction with respect to the foot component.

9. A prosthetic foot and ankle assembly according to claim 1, wherein said joint mechanism comprises a hydraulic linear piston and cylinder assembly and a valve arrangement con-

12

trolling the flow of hydraulic fluid between chambers of the piston and cylinder assembly on opposite sides of the piston thereof, the valve arrangement allowing individual setting of dorsi- and plantar-flexion damping resistances, and wherein the joint mechanism defines a medial-lateral joint flexion axis, and the joint flexion axis is to the anterior of the said central axis of the piston and cylinder assembly.

10. A prosthetic foot and ankle assembly according to claim 9, wherein said joint mechanism includes two passages in communication with a variable-volume chamber of the piston and cylinder assembly, each passage containing a respective non-return valve, one oriented to prevent the flow of fluid from the chamber through its respective passage and the other oriented to prevent the admission of fluid to the chamber through the other passage.

11. A prosthetic foot and ankle assembly according to claim 10, including an adjustable damping orifice in at least one of the two passages.

12. A prosthetic foot and ankle assembly according to claim 10, including an adjustable damping orifice that forms part of a passage in communication with the chamber and through which fluid flows during flexion of the ankle joint in a dorsi direction.

13. A prosthetic foot and ankle assembly according to claim 12, wherein said joint mechanism includes a flexion limiter limiting dorsi-flexion of the joint mechanism to a dorsi-flexion limit, and wherein the adjustable damping orifice has a dorsi-flexion orifice area that is variable according to joint flexion, the area reducing as dorsi-flexion of the joint mechanism approaches the dorsi-flexion limit.

14. A prosthetic foot and ankle assembly according to claim 12, including a second adjustable damping orifice through which fluid flows during flexion of the joint mechanism in a plantar direction.

15. A prosthetic foot and ankle assembly according to claim 1, wherein said joint mechanism includes a flexion limiter limiting dorsi-flexion of the joint mechanism to a dorsi-flexion limit, the assembly including a cushioning device for increasing resistance to dorsi-flexion as flexion of the ankle joint approaches said dorsi-flexion limit.

16. A lower limb prosthesis comprising:

a shin component defining a shin axis,

a foot component, and

a prosthetic ankle joint comprising a mechanism providing resistance to ankle flexion, wherein the mechanism is constructed and arranged such that said resistance is predominantly provided by hydraulic damping whenever the ankle joint is flexed in both dorsi- and plantar-flexion directions, said ankle joint coupling the shin component to the foot component,

wherein at least one of the foot component and the shin component includes a resilient section allowing resilient dorsi-flexion of at least an anterior portion of the foot component relative to the shin axis.

17. A prosthesis according to claim 16, wherein the foot component comprises an energy-storing spring arranged to be deflected when a dorsi-flexion load is applied to the foot anterior portion.

18. A prosthesis according to claim 16, wherein the resilient section is associated with the coupling of the foot component and the ankle joint.

19. A prosthesis according to claim 16, wherein the resilient section is associated with the coupling of the shin component to the ankle joint.

20. A prosthetic foot/ankle assembly comprising the combination of (a) a prosthetic ankle joint comprising a mechanism providing resistance to ankle flexion, wherein the

13

mechanism is constructed and arranged such that said resistance is predominantly provided by hydraulic damping whenever the ankle joint is flexed in both dorsi- and plantar-flexion directions, and (b) a prosthetic foot having an anterior portion, a posterior portion and an ankle-mounting portion, wherein the assembly constitutes a Maxwell-model damper/spring combination comprising a damper element and a spring element, wherein the damper element is said ankle joint and the spring element is a spring component arranged in series with the ankle joint.

21. An assembly according to claim 20, wherein the spring component is located distally of said ankle joint.

22. An assembly according to claim 20, wherein the spring component is a leaf spring supporting the anterior portion of the foot on the ankle-mounting portion thereof.

* * * * *

14